

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111324\
 Data File : BE101594.D
 Acq On : 13 Nov 2024 14:18
 Operator : RC/JU
 Sample : PB164886TB
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB164886TB

Quant Time: Nov 13 15:19:59 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 07 00:01:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.547	152	24490	20.000	ng	-0.02
21) Naphthalene-d8	10.320	136	91803	20.000	ng	#-0.01
39) Acenaphthene-d10	14.168	164	60942	20.000	ng	0.00
64) Phenanthrene-d10	16.912	188	150693	20.000	ng	0.00
76) Chrysene-d12	21.084	240	189992	20.000	ng	0.00
86) Perylene-d12	23.364	264	287050	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.302	112	66535	48.038	ng	-0.01
7) Phenol-d6	6.936	99	186476	98.197	ng	-0.01
23) Nitrobenzene-d5	8.757	82	182465	125.545	ng	-0.02
42) 2,4,6-Tribromophenol	15.678	330	130671	113.950	ng	0.00
45) 2-Fluorobiphenyl	12.788	172	409704	109.771	ng	-0.01
79) Terphenyl-d14	19.503	244	980212	114.203	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111324\
Data File : BE101594.D
Acq On : 13 Nov 2024 14:18
Operator : RC/JU
Sample : PB164886TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164886TB

Quant Time: Nov 13 15:19:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

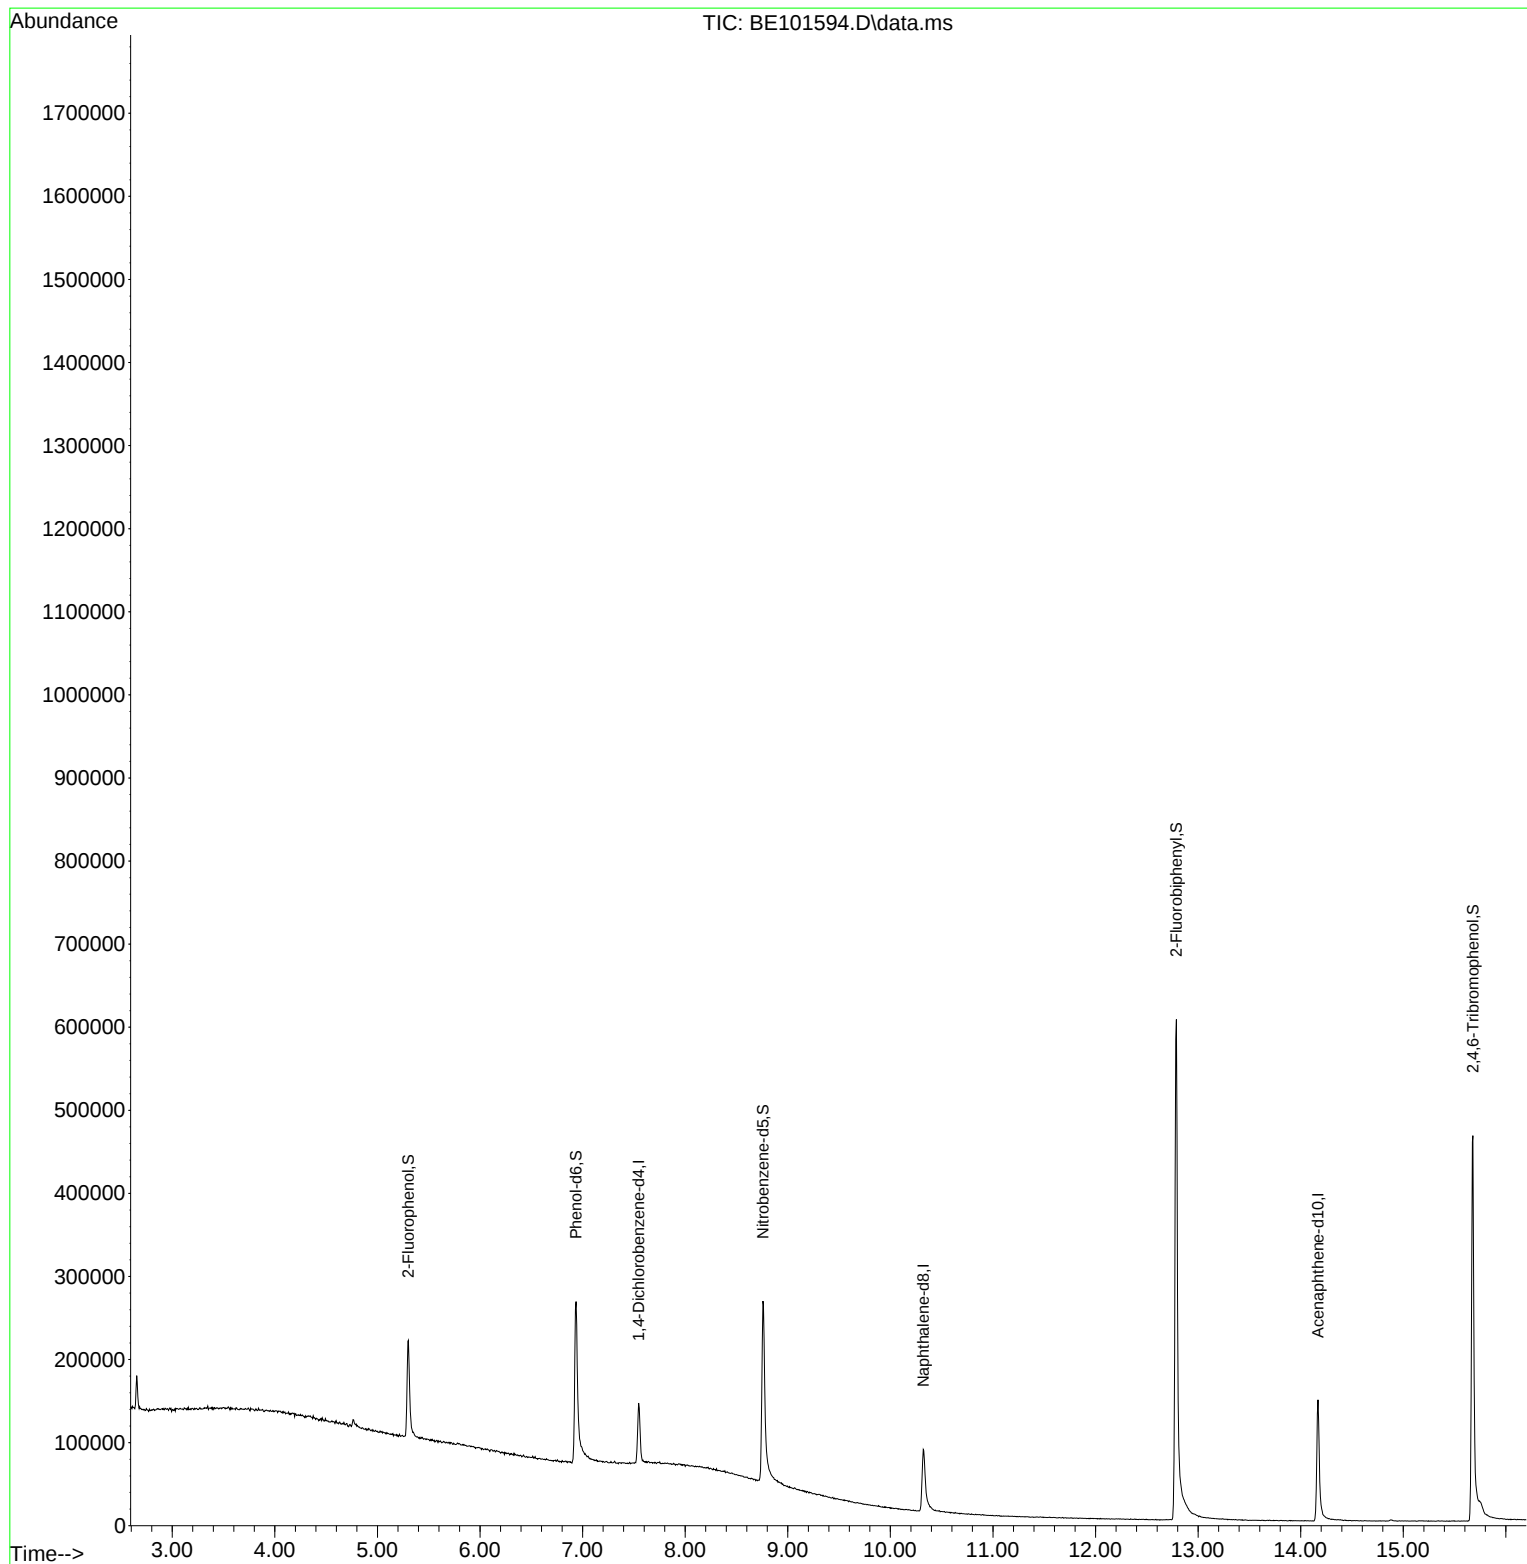

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111324\
Data File : BE101594.D
Acq On : 13 Nov 2024 14:18
Operator : RC/JU
Sample : PB164886TB
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB164886TB

Quant Time: Nov 13 15:19:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

