
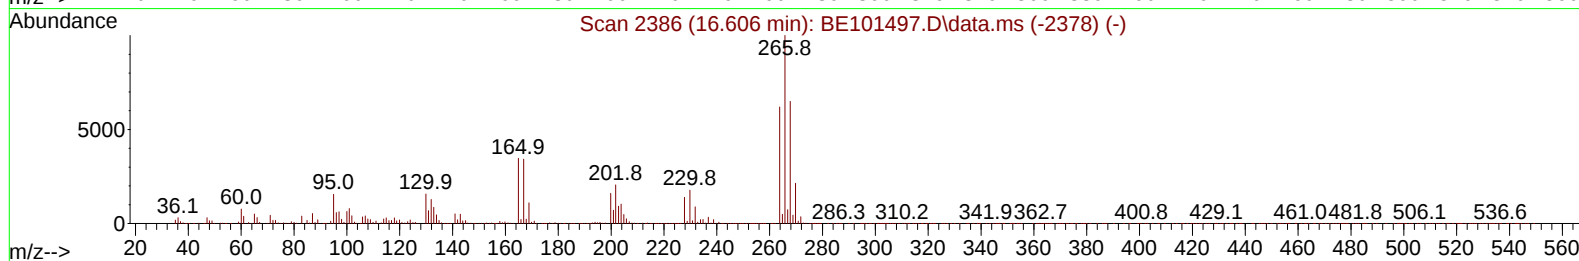
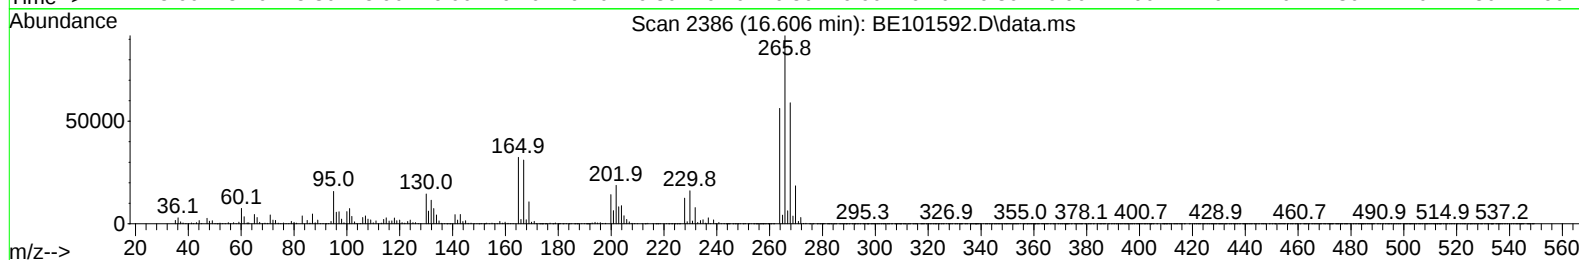


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111324\
Data File : BE101592.D
Acq On : 13 Nov 2024 12:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 13:00:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

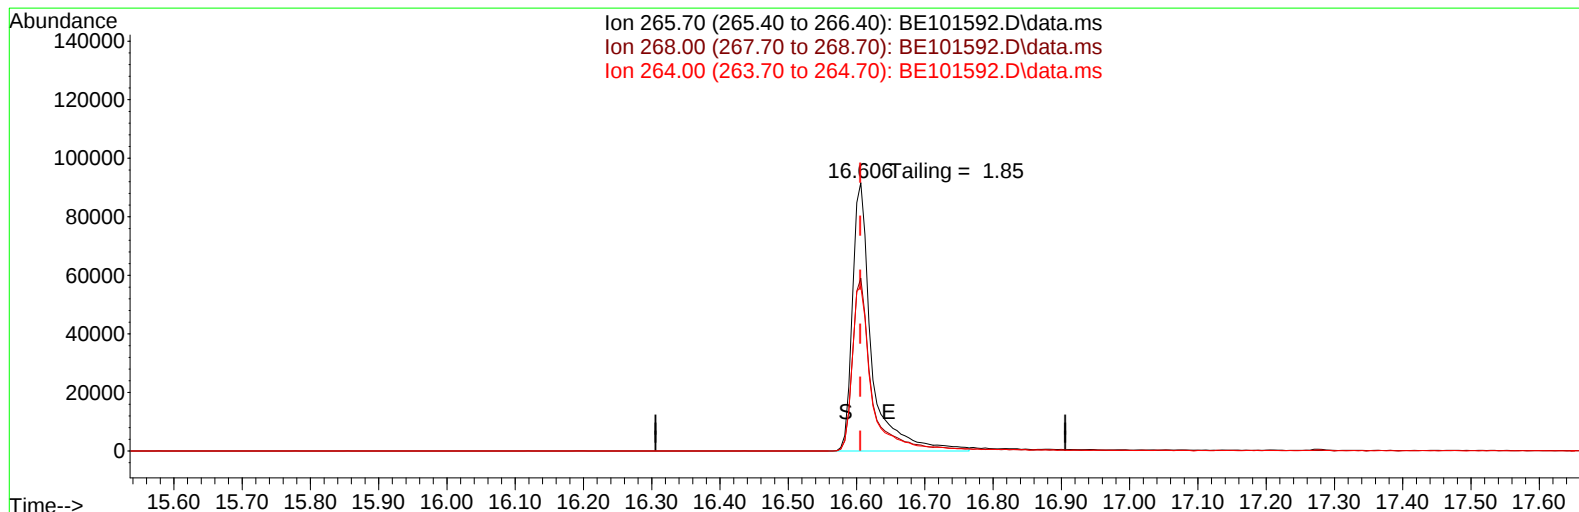

TIC: BE101592.D\data.ms

(70) Pentachlorophenol (C)




16.606min (+ 0.001) 897781.18 ng

response 141416

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	64.34
264.00	62.00	61.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111324\
Data File : BE101592.D
Acq On : 13 Nov 2024 12:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 13:00:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

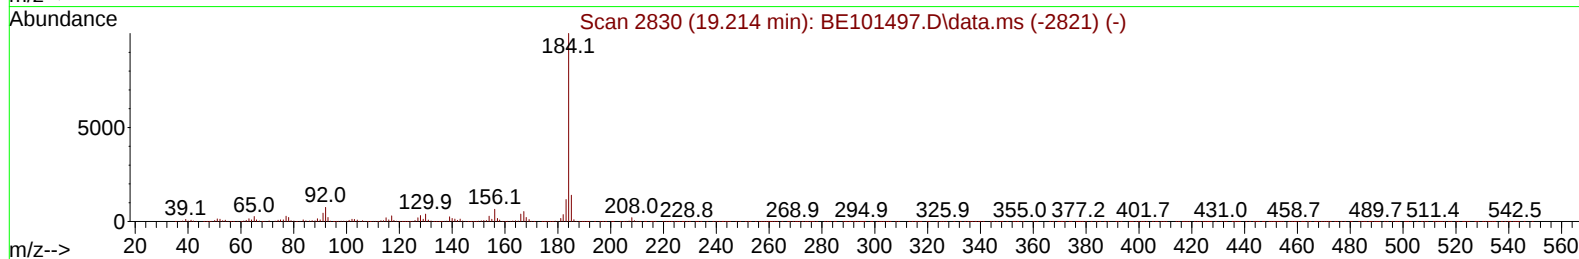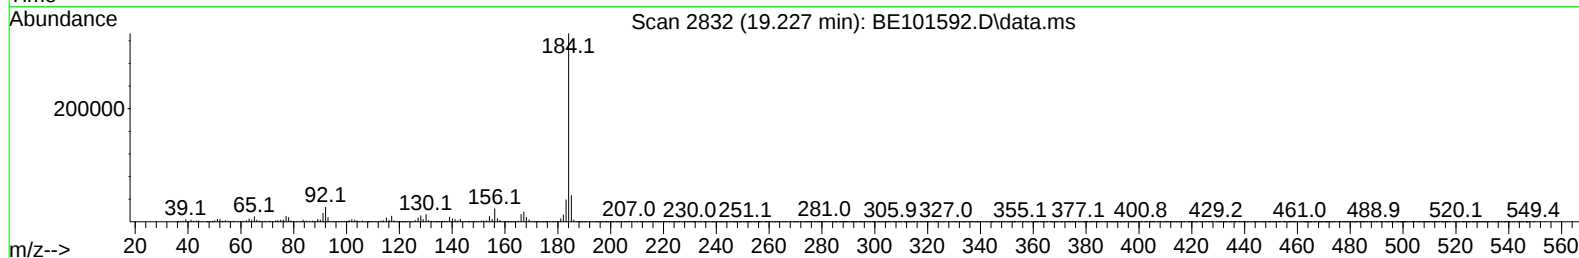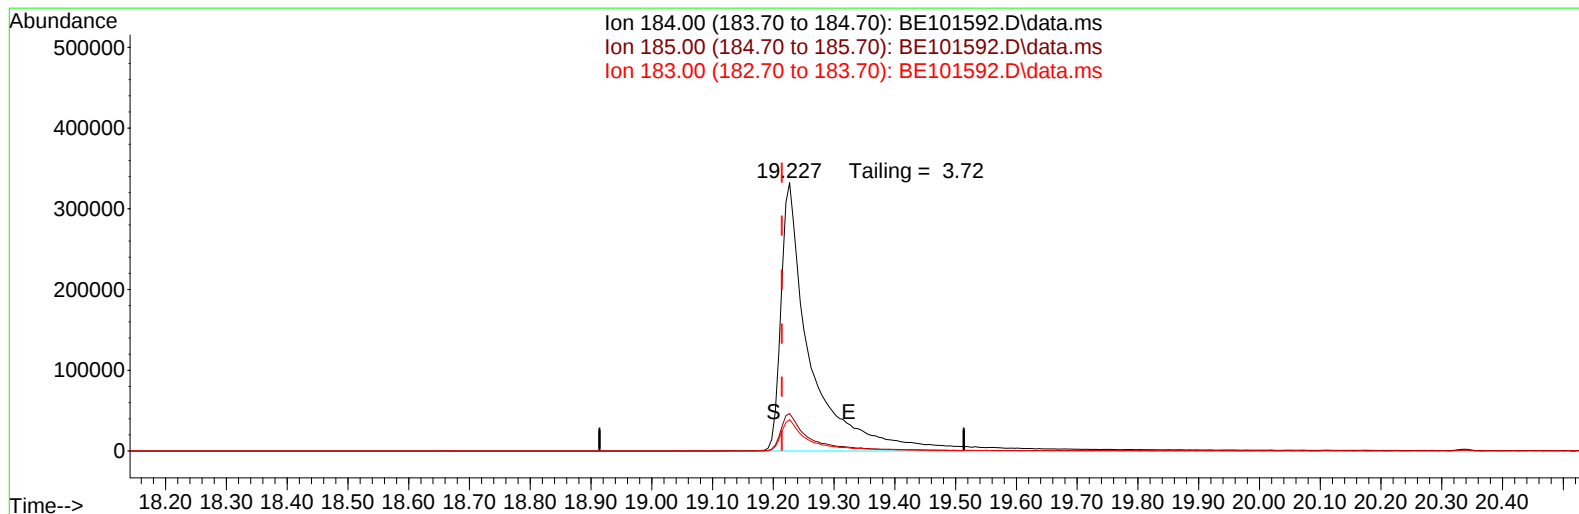

TIC: BE101592.D\data.ms

(77) Benzidine**19.227min (+ 0.013) 1362743.89 ng m****response 1112376**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.94
183.00	11.70	11.70
0.00	0.00	0.00