
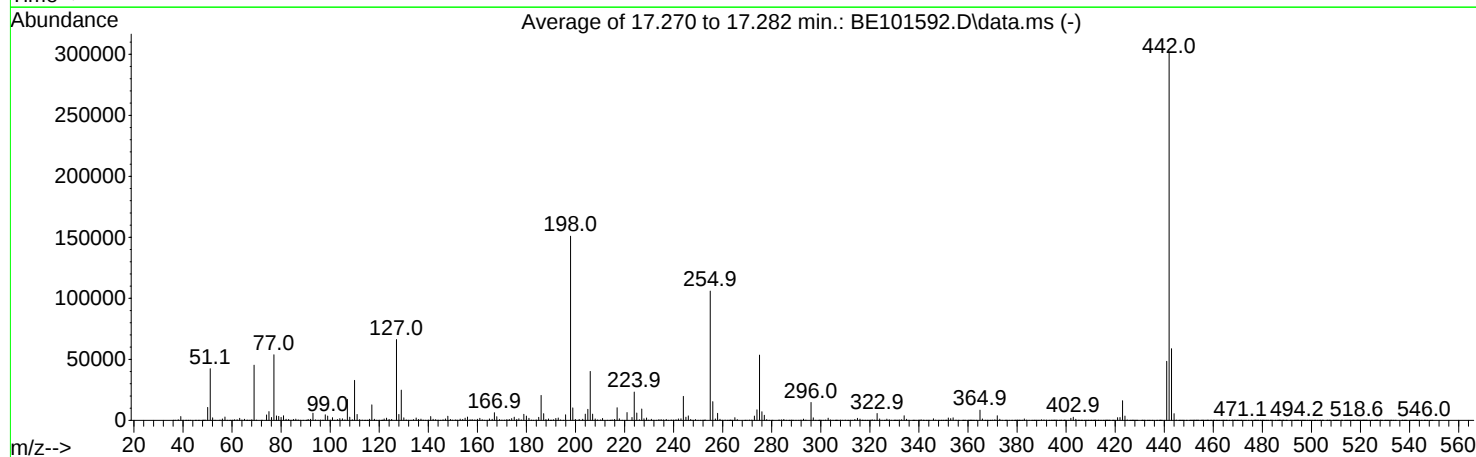


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111324\
Data File : BE101592.D
Acq On : 13 Nov 2024 12:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 07 00:01:20 2024

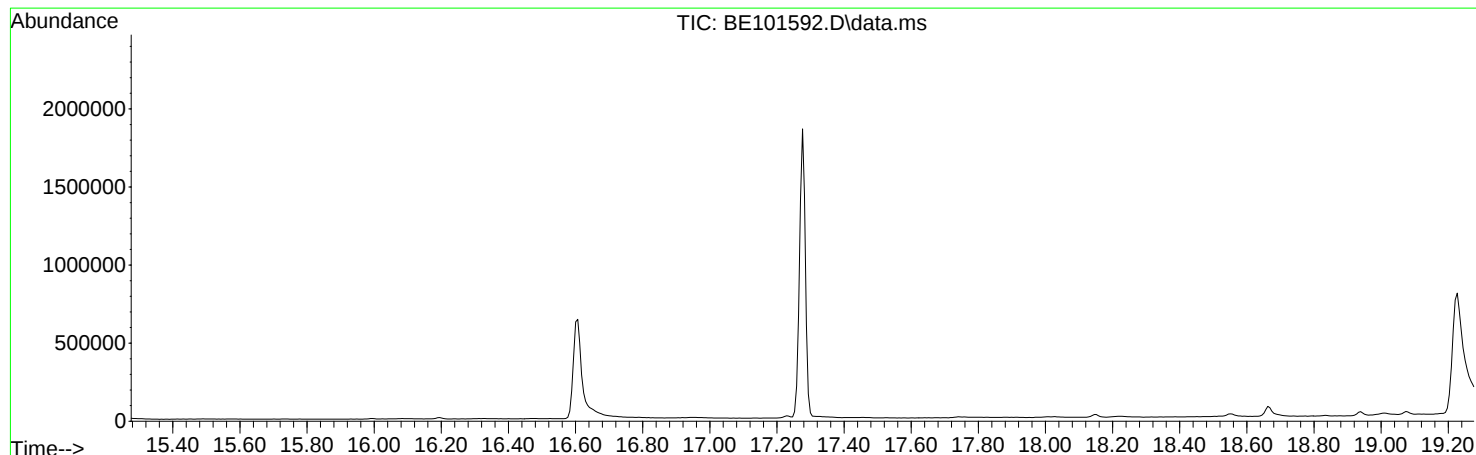




AutoFind: Scans 2499, 2500, 2501; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	42430	PASS
68	69	0.00	2	1.1	482	PASS
69	198	0.00	100	30.0	45239	PASS
70	69	0.00	2	0.5	241	PASS
127	198	10	80	43.9	66204	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	150898	PASS
199	198	5	9	6.7	10182	PASS
275	198	10	60	35.5	53581	PASS
365	198	1	100	5.6	8449	PASS
441	198	0.01	100	32.1	48407	PASS
442	442	50	100	100.0	301483	PASS
443	442	15	24	19.5	58742	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111324\
Data File : BE101592.D
Acq On : 13 Nov 2024 12:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 13 13:00:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

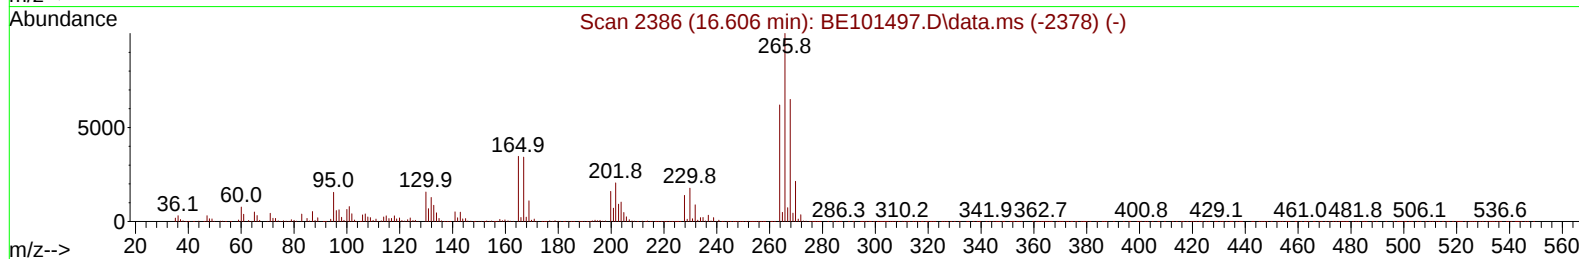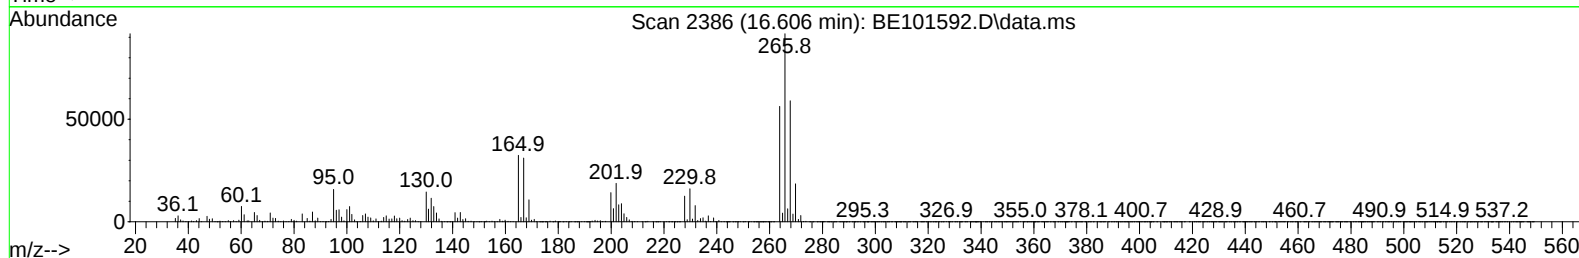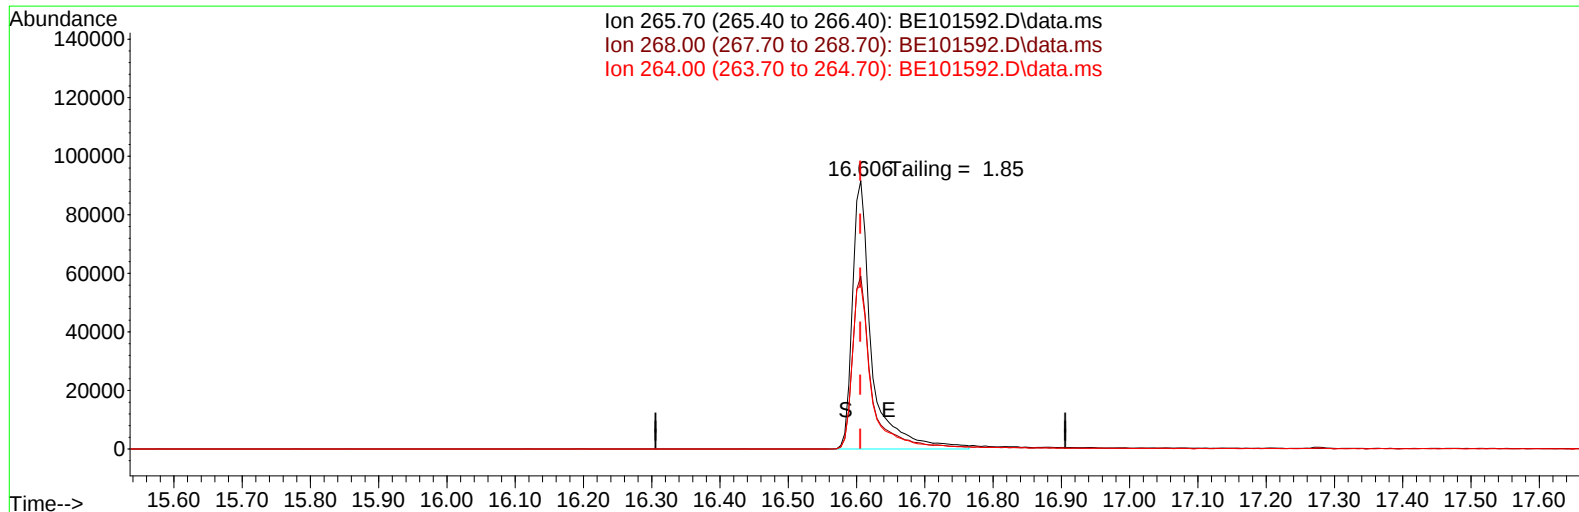

TIC: BE101592.D\data.ms

(70) Pentachlorophenol (C)

16.606min (+ 0.001) 897781.18 ng




response 141416

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	64.34
264.00	62.00	61.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE111324\
Data File : BE101592.D
Acq On : 13 Nov 2024 12:30
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Quant Time: Nov 13 13:00:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-BE110624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 07 00:01:20 2024
Response via : Initial Calibration

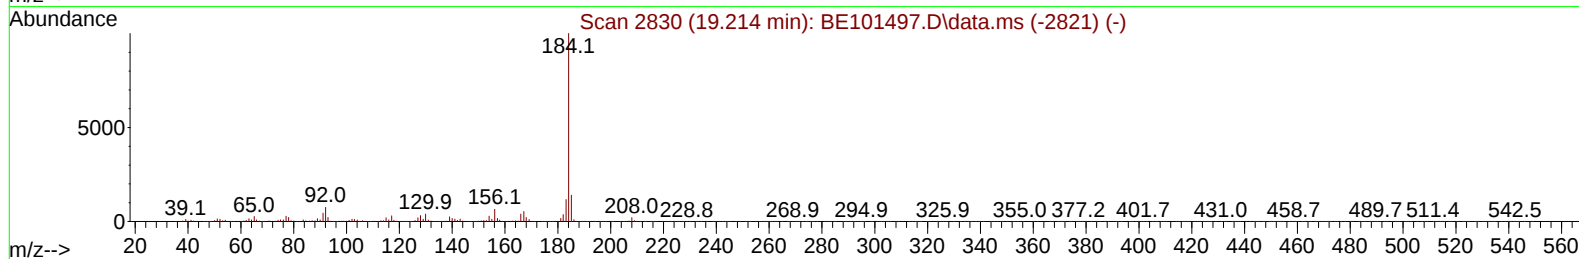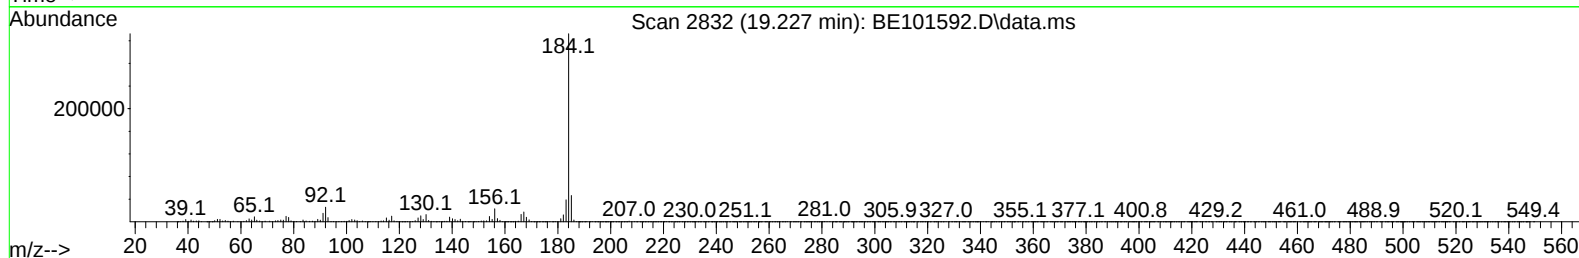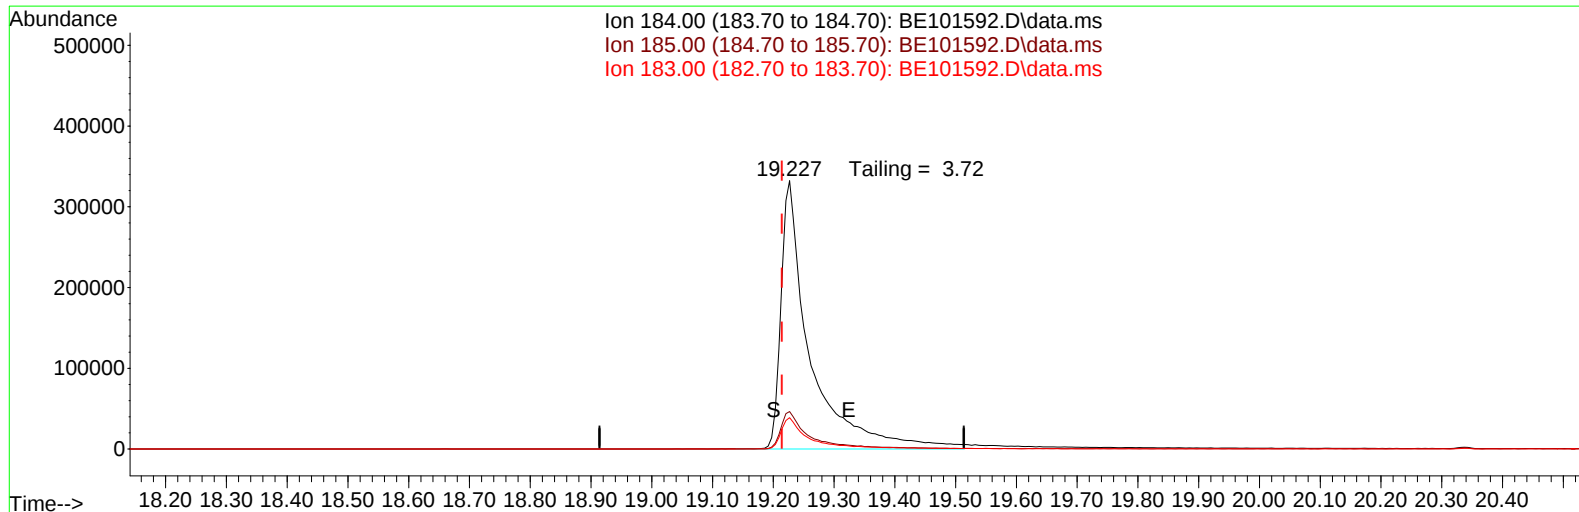

TIC: BE101592.D\data.ms

(77) Benzidine

19.227min (+ 0.013) 1362743.89 ng m

response 1112376

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.94
183.00	11.70	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2024	BNA_E	<u>BE101592.D</u>
Compound Name	Response	Retention Time
DDT	626414	20.337
DDD	18986	19.908
DDE	255	19.397
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19241	645655	2.98

Instrument :
BNA_E
ClientSampleId :
DFTPP