


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE050619\
 Data File : BE099547.D
 Acq On : 6 May 2019 11:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE042919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 07 06:25:51 2019

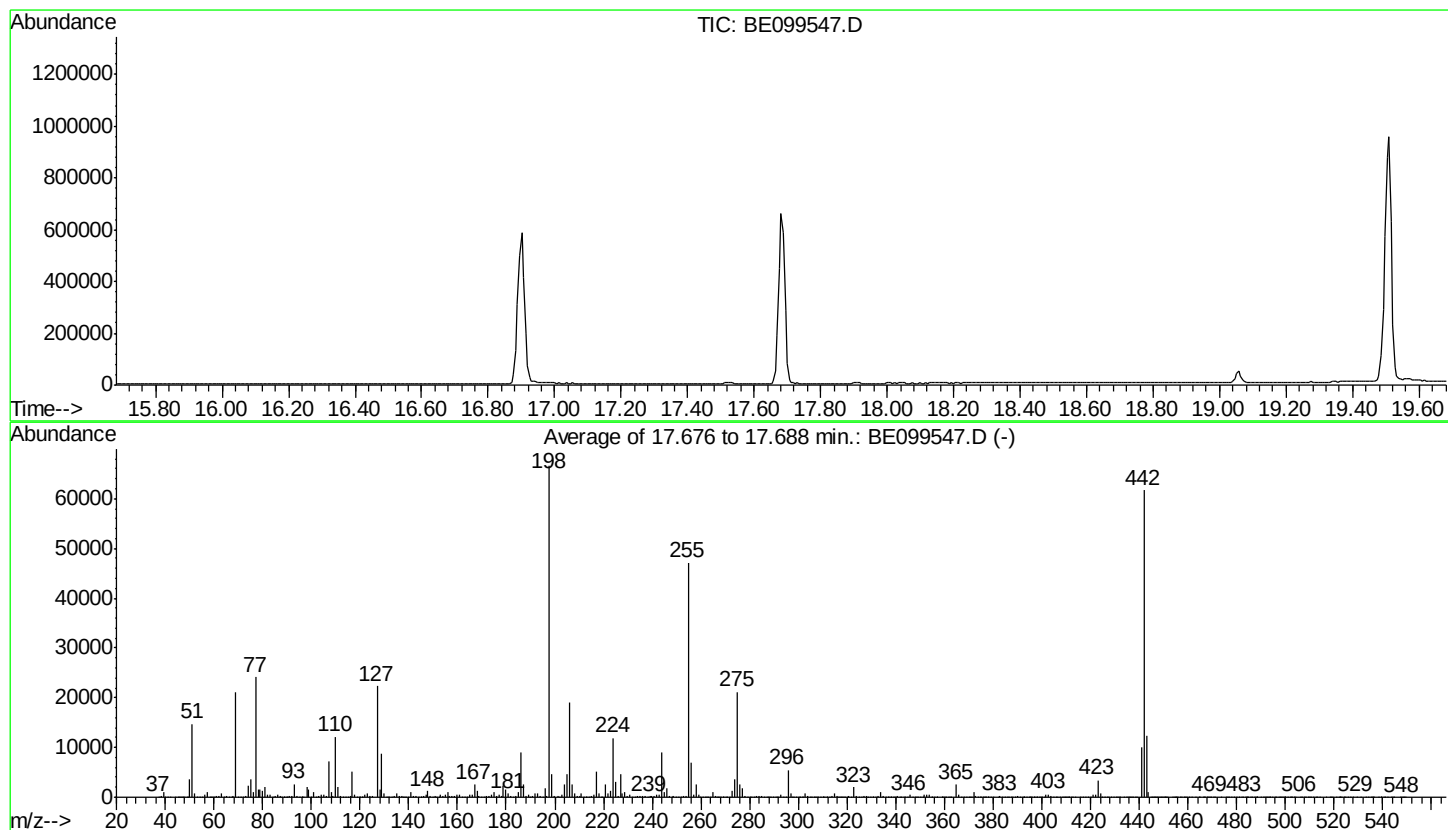

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	14796	PASS
68	69	0.00	2	1.2	247	PASS
69	198	0.00	100	31.5	20988	PASS
70	69	0.00	2	0.5	104	PASS
127	198	10	80	33.6	22375	PASS
197	198	0.00	2	0.3	202	PASS
198	198	100	100	100.0	66640	PASS
199	198	5	9	6.8	4557	PASS
275	198	10	60	31.7	21106	PASS
365	198	1	100	3.7	2471	PASS
441	198	0.01	100	15.2	10113	PASS
442	198	50	100	92.6	61729	PASS
443	442	15	24	19.9	12279	PASS