


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE051719\
 Data File : BE099640.D
 Acq On : 17 May 2019 7:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE051419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 14 19:30:50 2019

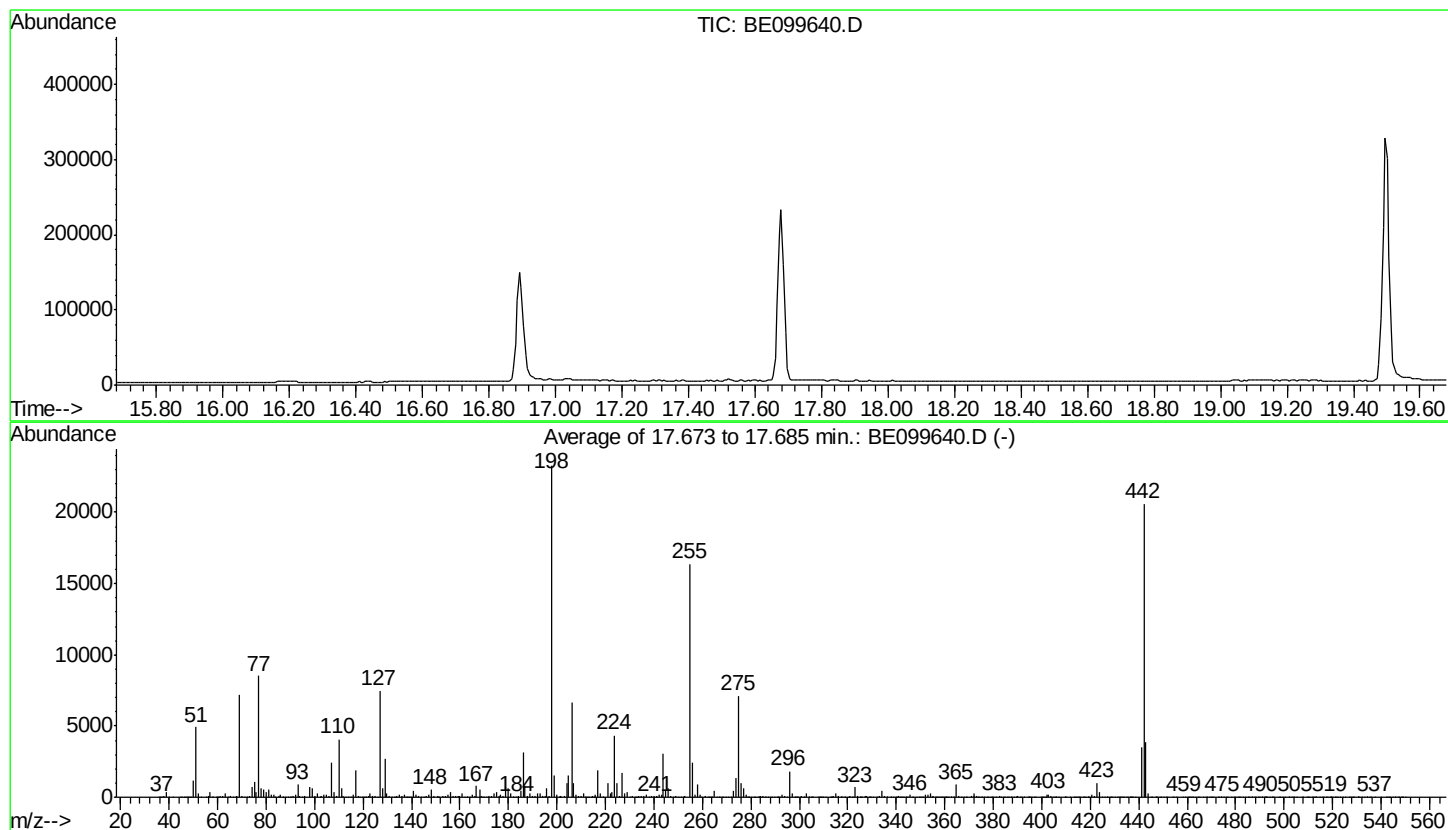

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.2	4936	PASS
68	69	0.00	2	0.9	65	PASS
69	198	0.00	100	31.0	7207	PASS
70	69	0.00	2	0.7	53	PASS
127	198	10	80	32.2	7506	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23281	PASS
199	198	5	9	6.7	1564	PASS
275	198	10	60	30.6	7132	PASS
365	198	1	100	3.7	867	PASS
441	198	0.01	100	15.0	3500	PASS
442	198	50	100	88.5	20613	PASS
443	442	15	24	18.9	3895	PASS