


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060519\
 Data File : BE099796.D
 Acq On : 5 Jun 2019 8:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 05 14:35:58 2019

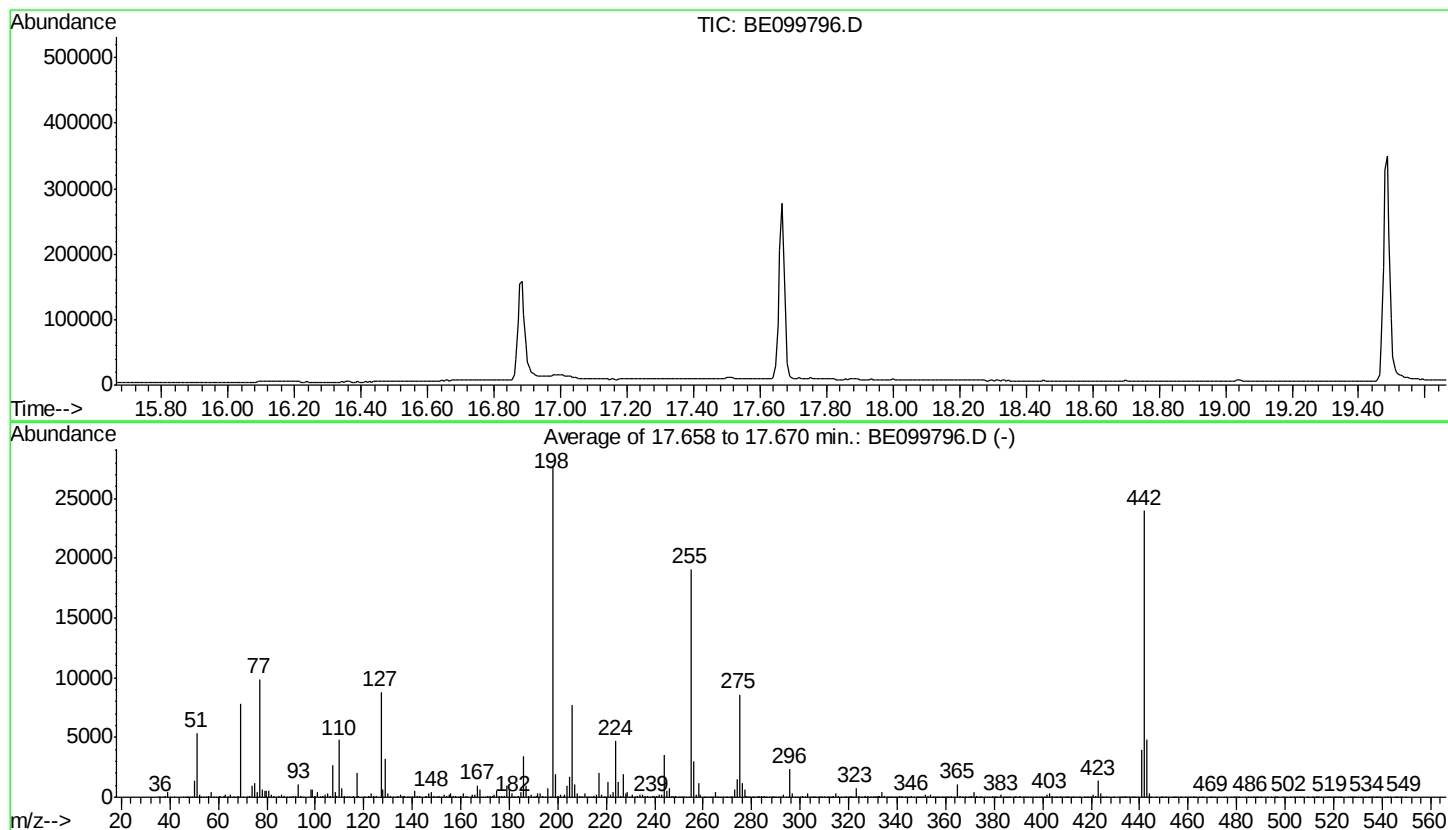

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2556

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.4	5390	PASS
68	69	0.00	2	1.2	91	PASS
69	198	0.00	100	28.2	7827	PASS
70	69	0.00	2	0.6	48	PASS
127	198	10	80	31.8	8821	PASS
197	198	0.00	2	0.2	44	PASS
198	198	100	100	100.0	27765	PASS
199	198	5	9	7.1	1965	PASS
275	198	10	60	31.0	8596	PASS
365	198	1	100	3.9	1095	PASS
441	198	0.01	100	14.4	4007	PASS
442	198	50	100	86.3	23969	PASS
443	442	15	24	20.0	4799	PASS