


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE060519\
 Data File : BE099807.D
 Acq On : 5 Jun 2019 17:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE060519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 05 14:35:58 2019

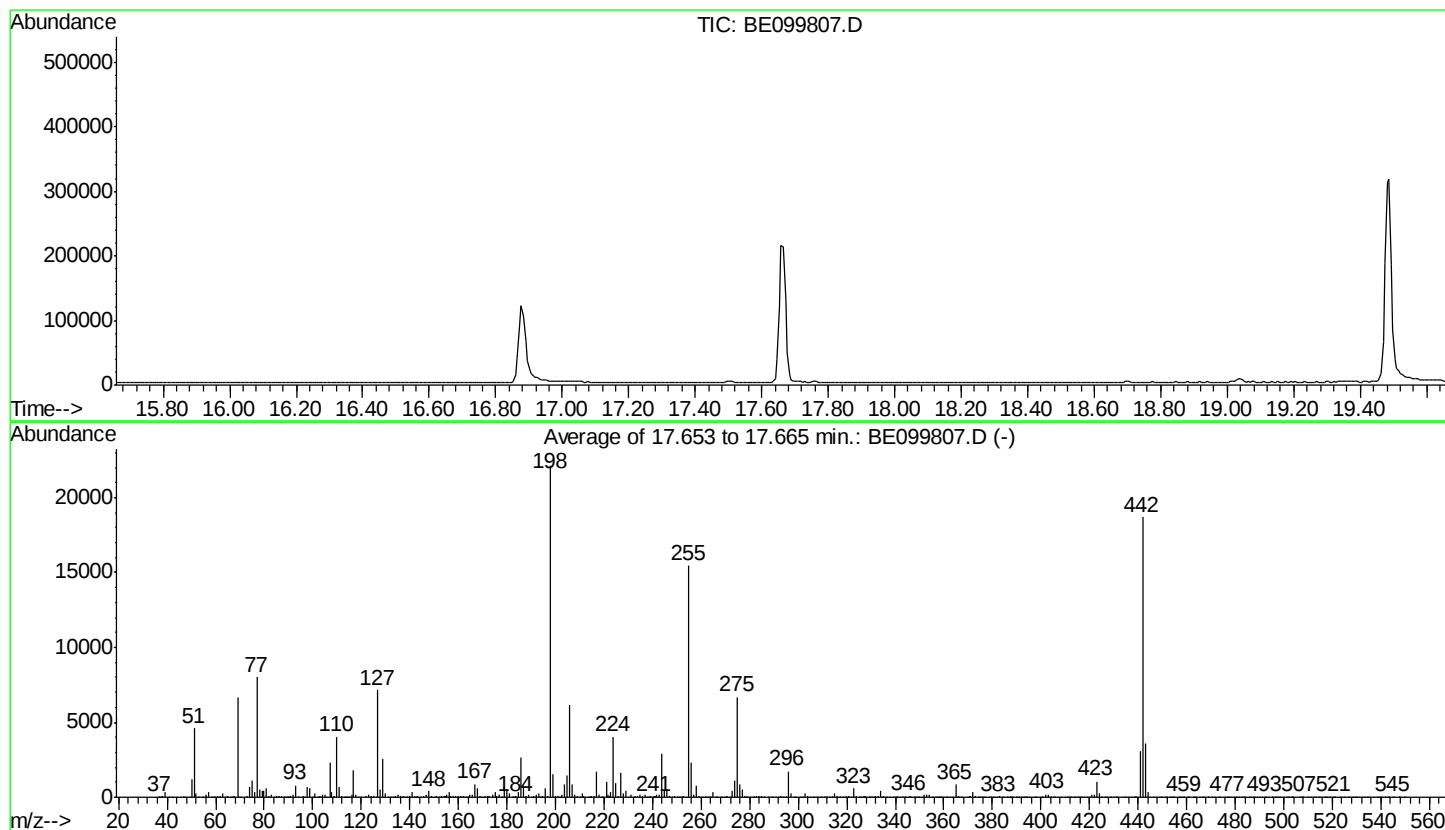

AutoFind: Scans 2564, 2565, 2566; Background Corrected with Scan 2555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.7	4575	PASS
68	69	0.00	2	1.4	93	PASS
69	198	0.00	100	30.3	6708	PASS
70	69	0.00	2	0.3	23	PASS
127	198	10	80	32.4	7174	PASS
197	198	0.00	2	0.3	74	PASS
198	198	100	100	100.0	22130	PASS
199	198	5	9	7.0	1553	PASS
275	198	10	60	30.2	6693	PASS
365	198	1	100	3.8	831	PASS
441	198	0.01	100	13.7	3037	PASS
442	198	50	100	84.4	18677	PASS
443	442	15	24	19.3	3599	PASS