

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070819\
 Data File : BF115405.D
 Acq On : 8 Jul 2019 15:01
 Operator : HP/JU
 Sample : PB121130BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB121130BL

Quant Time: Jul 08 16:55:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 05 14:57:35 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	215834	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	857344	20.00	ng	0.00
39) Acenaphthene-d10	9.93	164	429805	20.00	ng	0.00
64) Phenanthrene-d10	11.42	188	840561	20.00	ng	0.00
76) Chrysene-d12	14.06	240	604848	20.00	ng	-0.01
87) Perylene-d12	15.56	264	543523	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	1543437	110.49	ng	0.02
7) Phenol-d6	6.53	99	1999757	112.56	ng	0.00
23) Nitrobenzene-d5	7.46	82	1283472	88.45	ng	0.00
42) 2,4,6-Tribromophenol	10.72	330	573301	120.64	ng	0.00
45) 2-Fluorobiphenyl	9.26	172	2209034	90.19	ng	0.00
79) Terphenyl-d14	13.00	244	2527486	85.56	ng	0.00
Target Compounds						
9) Benzaldehyde	6.53	77	2972	Below Cal		Qvalue # 1
19) n-Nitroso-di-n-propylamine	7.46	70	174370	14.507	ng	# 77
25) Isophorone	7.46	82	1272671	40.463	ng	# 64
51) 2,6-Dinitrotoluene	9.93	165	55506	7.933	ng	# 23
57) 2,4-Dinitrotoluene	9.93	165	55506	6.243	ng	# 25
65) 4,6-Dinitro-2-methylphenol	10.72	198	1088	8.044	ng	# 1
67) 4-Bromophenyl-phenylether	10.72	248	34583	3.667	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070819\
Data File : BF115405.D
Acq On : 8 Jul 2019 15:01
Operator : HP/JU
Sample : PB121130BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB121130BL

Quant Time: Jul 08 16:55:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF070519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 05 14:57:35 2019
Response via : Initial Calibration

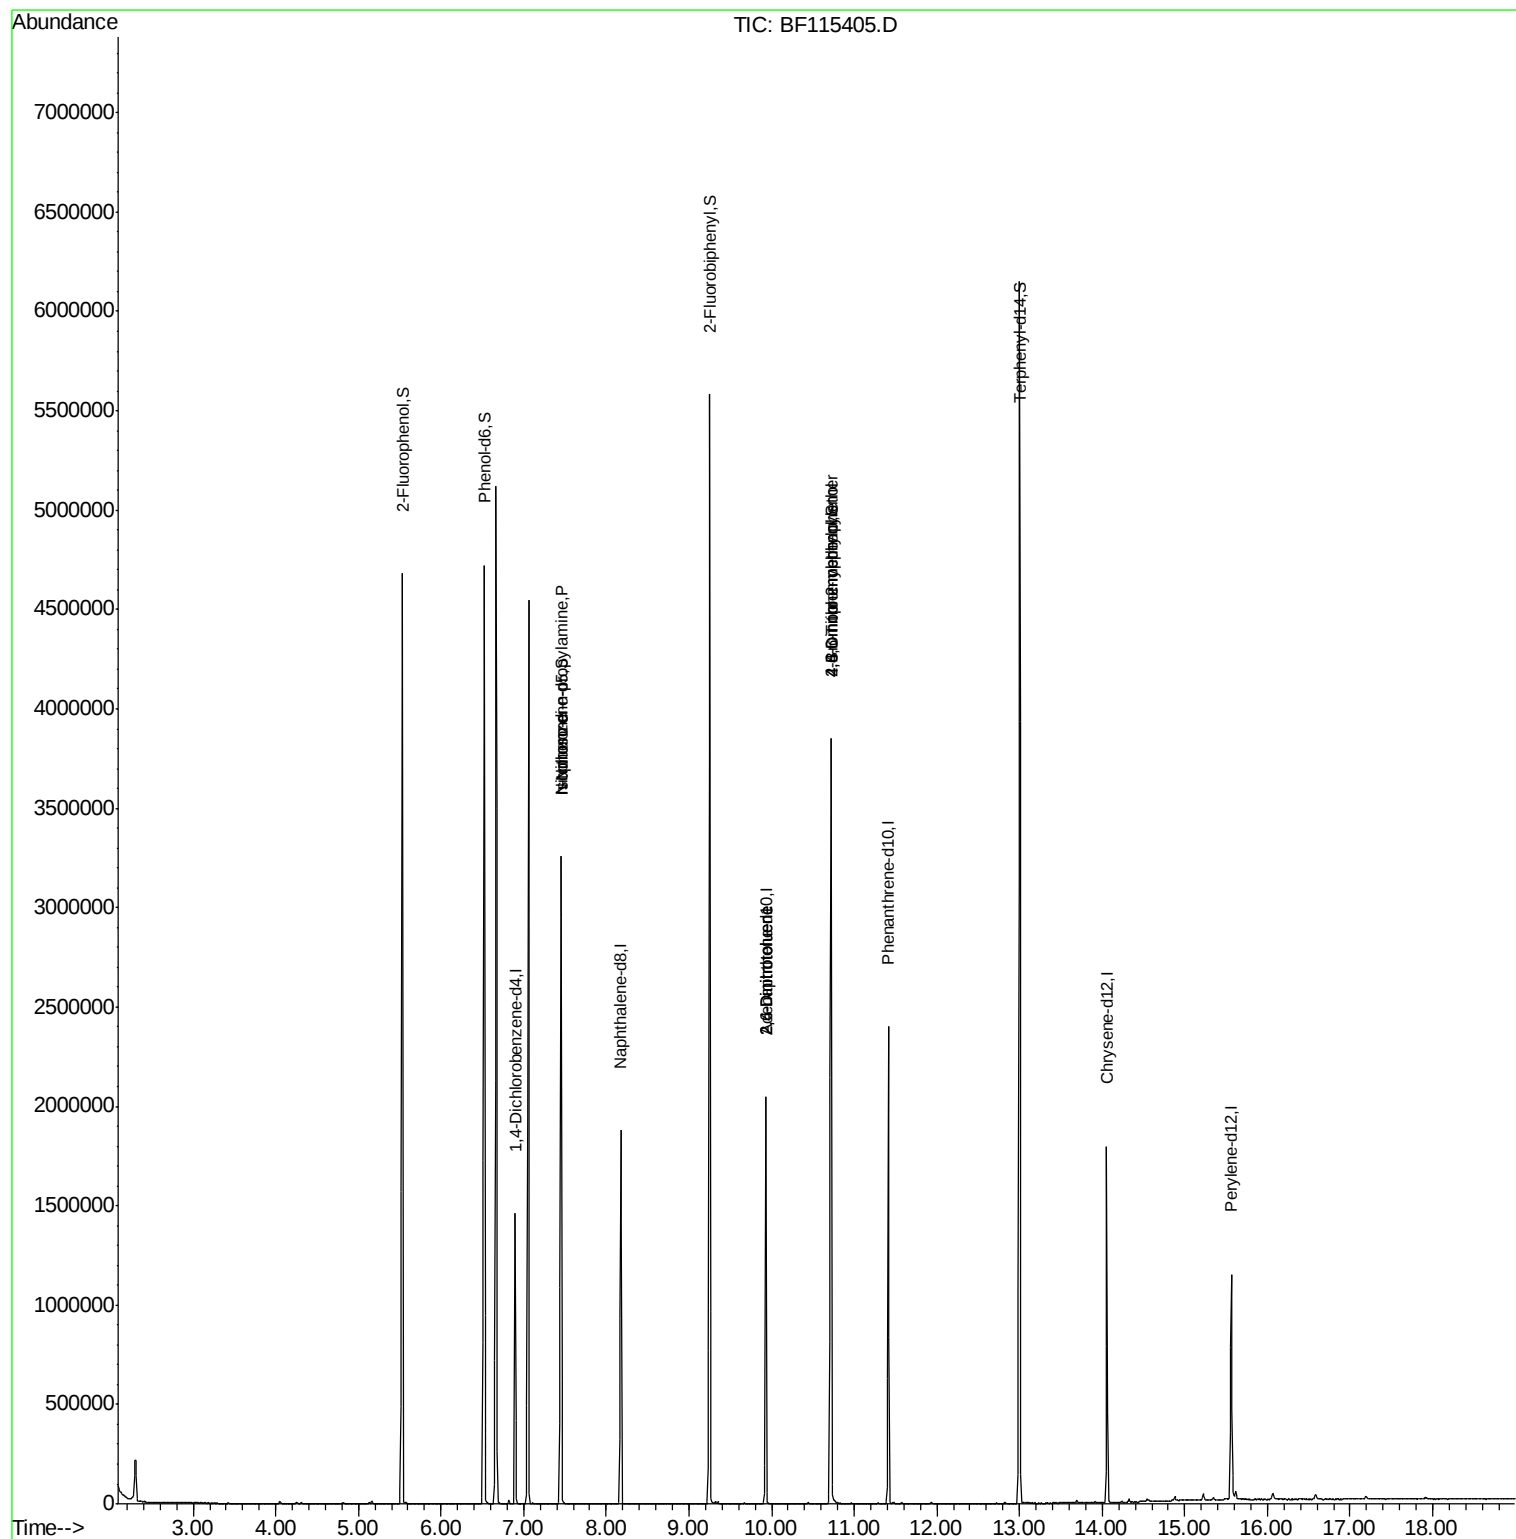







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.90 min Scan# 818
 Delta R.T. -0.00 min
 Lab File: BF115405.D
 Acq: 8 Jul 2019 15:01

Instrument :
 BNA_E
 ClientSampleId :
 PB121130BL

Tot Ion:152 Resp: 215834
 Ion Ratio Lower Upper
 152 100
 150 153.8 124.7 187.1
 115 59.7 48.1 72.1




Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

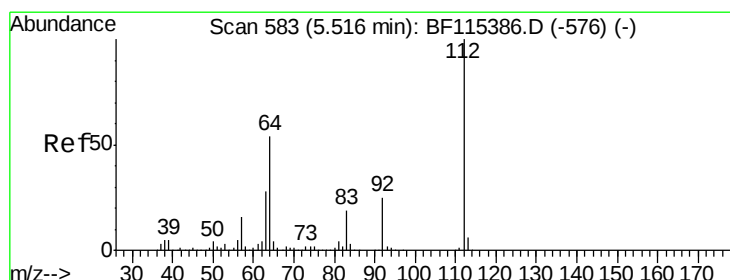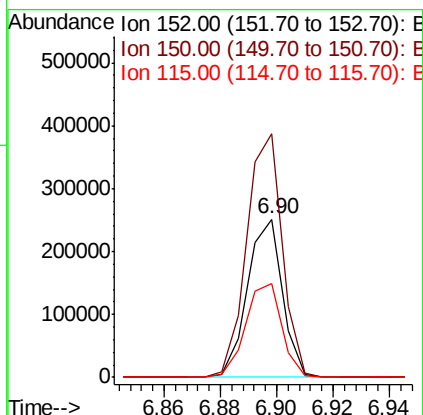




#5
 2-Fluorophenol
 Concen: 110.486 ng
 RT: 5.53 min Scan# 586
 Delta R.T. 0.02 min
 Lab File: BF115405.D
 Acq: 8 Jul 2019 15:01

Tgt Ion:112 Resp: 1543437
 Ion Ratio Lower Upper
 112 100
 64 56.1 43.0 64.6
 63 29.2 22.2 33.2



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

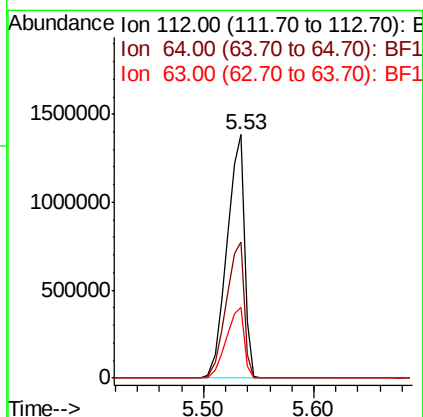

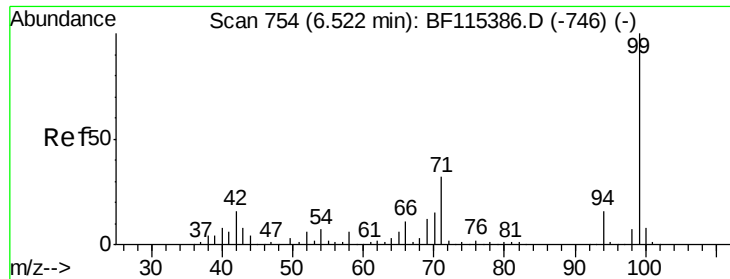

#7

Phenol-d6

Concen: 112.558 ng

RT: 6.53 min Scan# 755

Delta R.T. 0.01 min

Lab File: BF115405.D

Acq: 8 Jul 2019 15:01

Instrument :


BNA_E

ClientSampleId :

PB121130BL

Tot Ion: 99 Resp: 1999757

Ion	Ratio	Lower	Upper
99	100		
42	16.2	13.1	19.7
71	34.4	25.9	38.9






Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

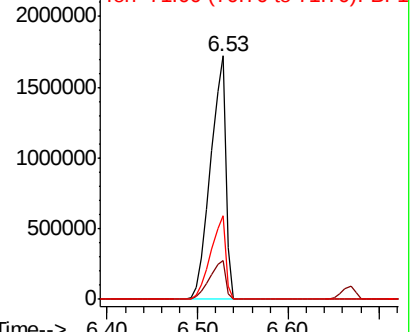

#9

Benzaldehyde

Concen: Below Cal

RT: 6.53 min Scan# 755


Delta R.T. 0.08 min

Lab File: BF115405.D

Acq: 8 Jul 2019 15:01

Tgt Ion: 77 Resp: 2972

Ion	Ratio	Lower	Upper
77	100		
105	0.0	79.0	119.0#
106	0.0	75.7	115.7#






Abundance

Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E




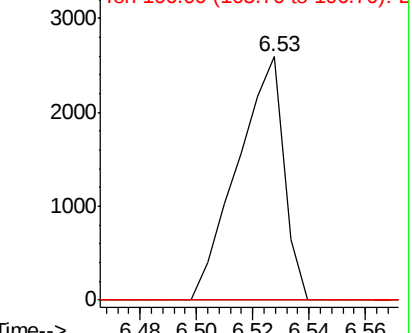


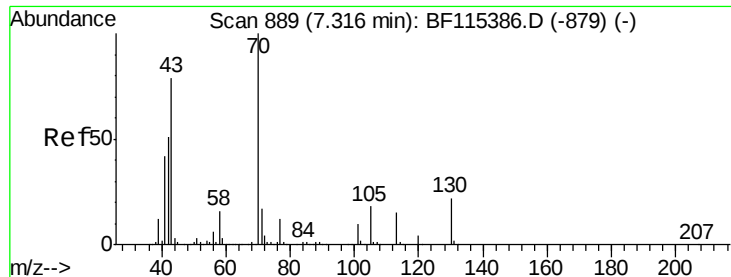

#19
n-Nitroso-di-n-propylamine
Concen: 14.507 ng
RT: 7.46 min Scan# 913
Delta R.T. 0.14 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01




Instrument :
BNA_E
ClientSampleId :
PB121130BL


Tot Ion: 70 Resp: 174370
Ion Ratio Lower Upper
70 100
42 41.5 41.1 61.7
101 0.0 8.0 12.0#
130 2.4 17.8 26.8#

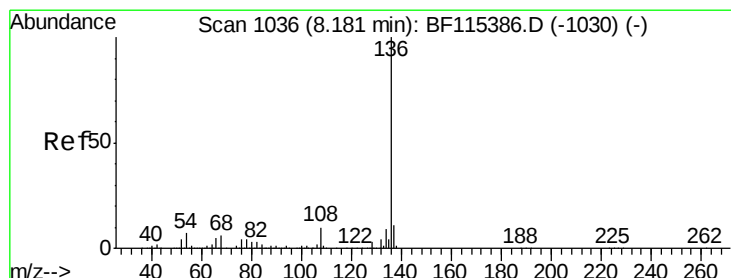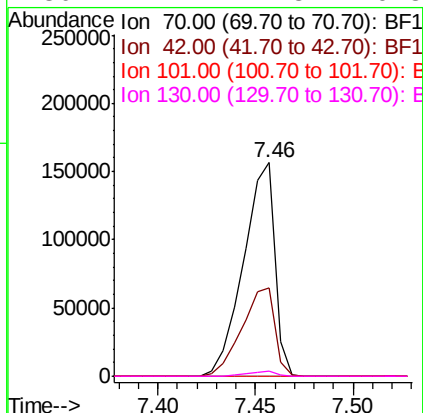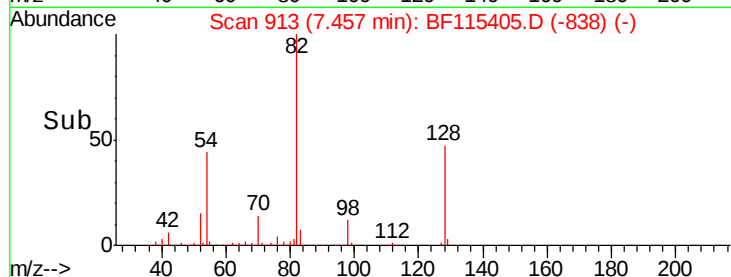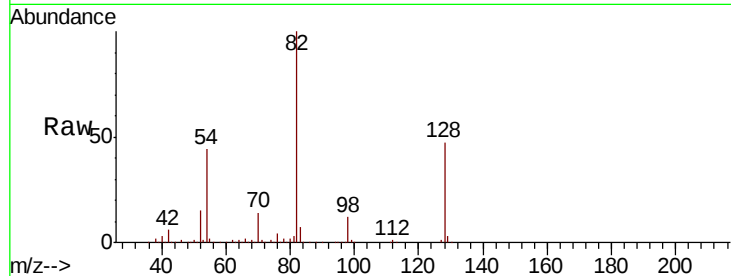

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.17 min Scan# 1035
Delta R.T. -0.01 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01

Tgt Ion: 136 Resp: 857344
Ion Ratio Lower Upper
136 100
137 11.3 8.9 13.3
54 7.4 5.6 8.4
68 6.6 4.9 7.3

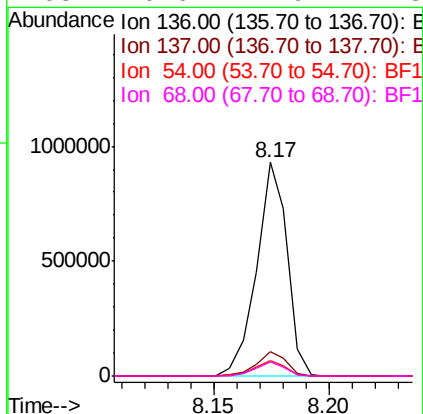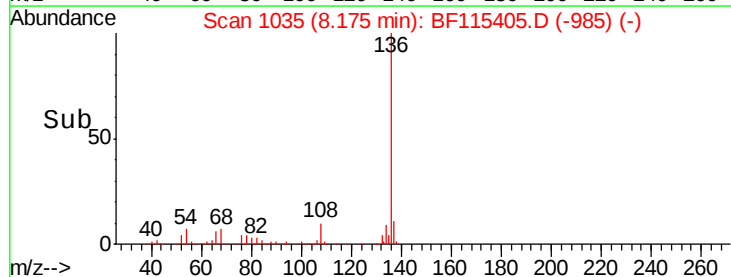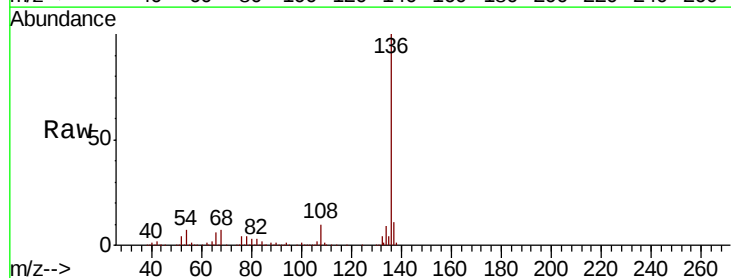







#23
Nitrobenzene-d5
Concen: 88.450 ng
RT: 7.46 min Scan# 913
Delta R.T. -0.00 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01

Instrument :
BNA_E
ClientSampleId :
PB121130BL

Tot Ion: 82 Resp: 1283472
Ion Ratio Lower Upper
82 100
128 47.4 35.7 53.5
54 44.1 36.3 54.5

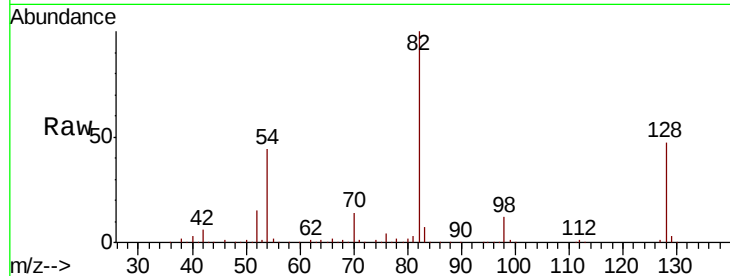


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1


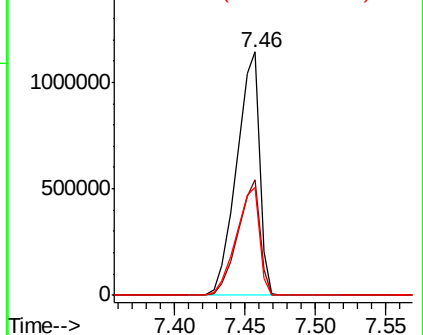



#25
Isophorone
Concen: 40.463 ng
RT: 7.46 min Scan# 913
Delta R.T. -0.26 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01

Tgt Ion: 82 Resp: 1272671
Ion Ratio Lower Upper
82 100
95 0.0 5.4 8.0#
138 0.0 14.9 22.3#



Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

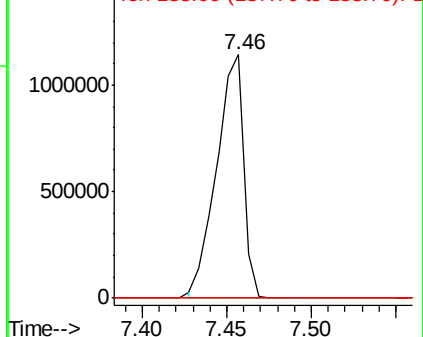


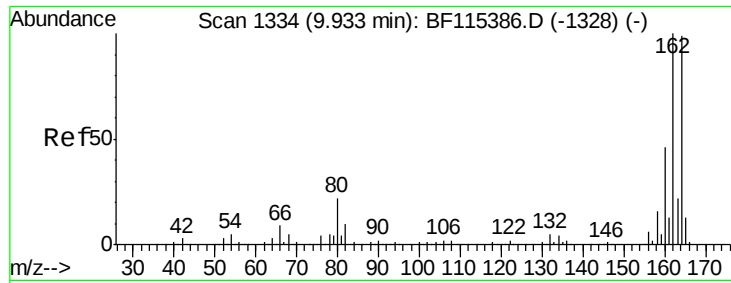




#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. -0.00 min
 Lab File: BF115405.D
 Acq: 8 Jul 2019 15:01

Instrument :
 BNA_E
 ClientSampleId :
 PB121130BL

Tot Ion:164 Resp: 429805
 Ion Ratio Lower Upper
 164 100
 162 104.9 80.6 121.0
 160 48.3 37.0 55.6

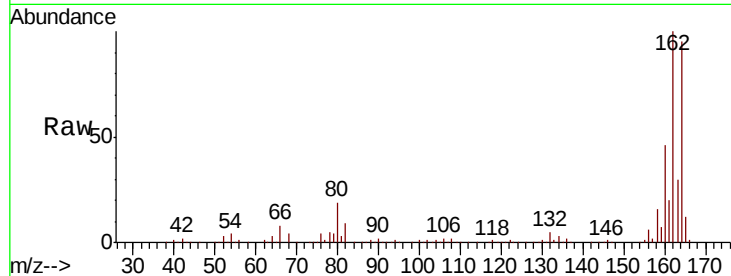


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

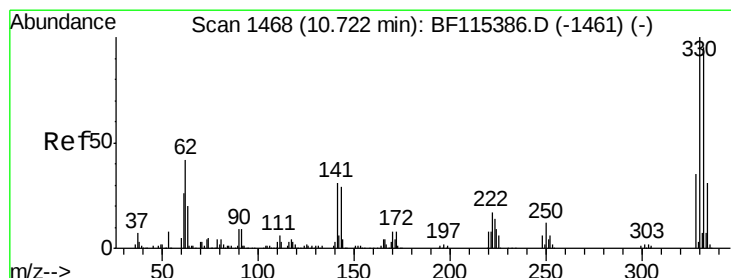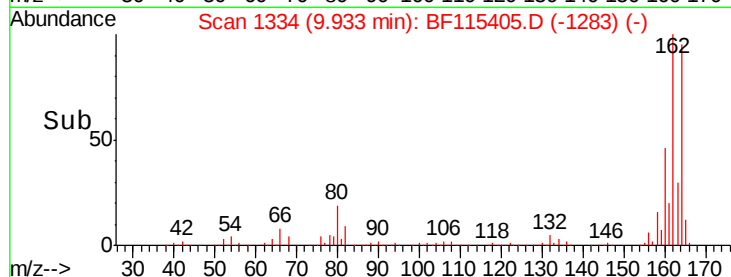
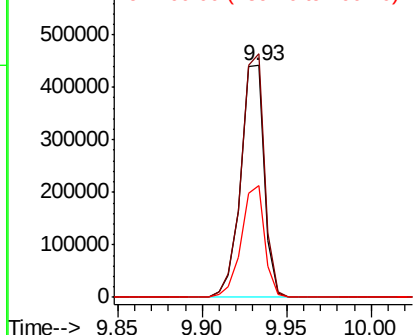



#42
 2,4,6-Tribromophenol
 Concen: 120.639 ng
 RT: 10.72 min Scan# 1468
 Delta R.T. -0.00 min
 Lab File: BF115405.D
 Acq: 8 Jul 2019 15:01

Tgt Ion:330 Resp: 573301
 Ion Ratio Lower Upper
 330 100
 332 95.9 76.3 114.5
 141 30.7 27.0 40.4

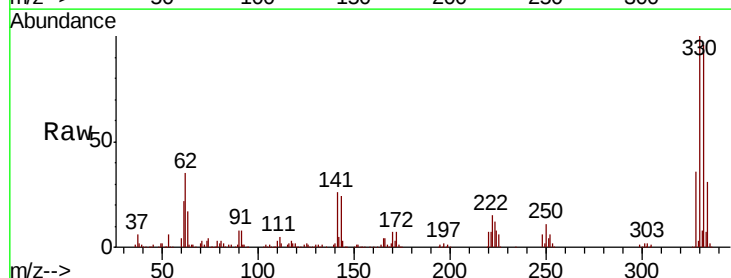

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

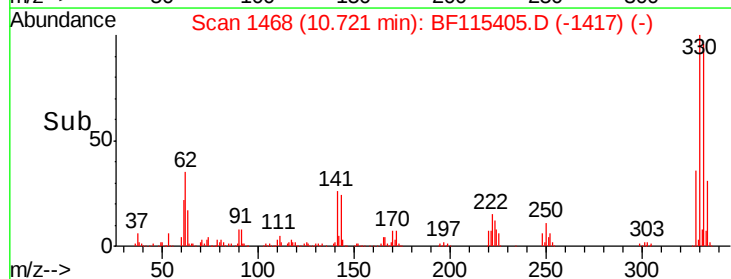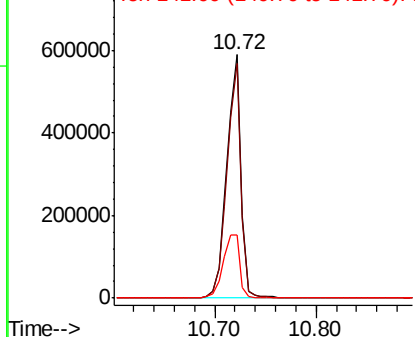


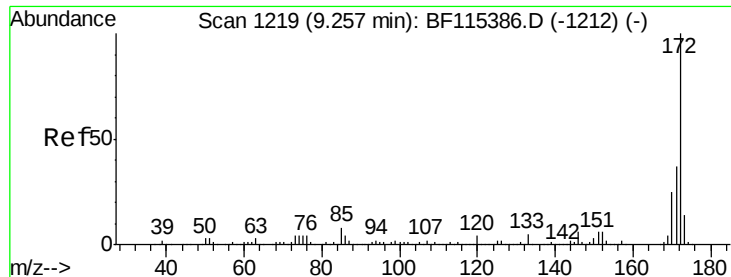




#45
2-Fluorobiphenyl
Concen: 90.187 ng
RT: 9.26 min Scan# 1219
Delta R.T. -0.00 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01

Instrument :
BNA_E
ClientSampleId :
PB121130BL

Tot Ion:172 Resp: 2209034
Ion Ratio Lower Upper
172 100
171 36.8 29.8 44.8
170 24.9 20.2 30.4

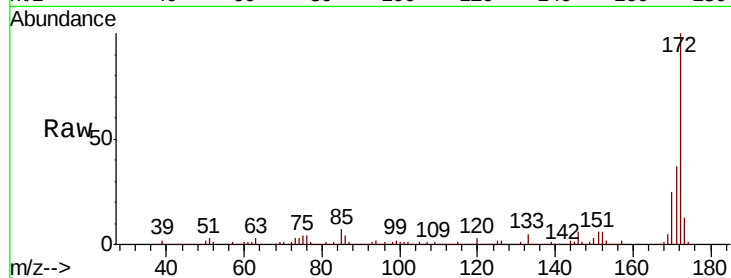


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

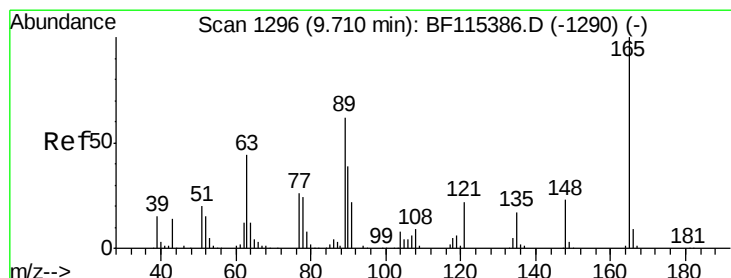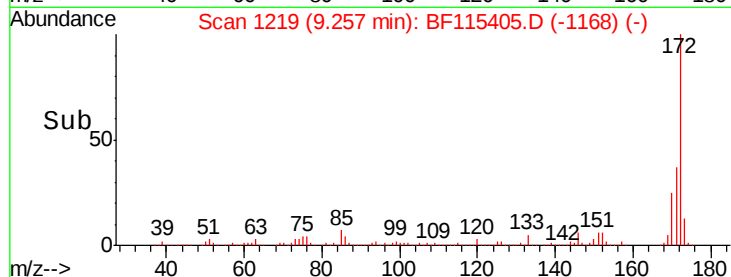
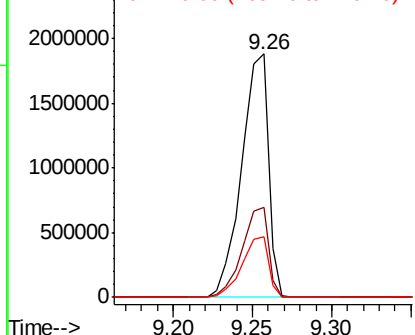



#51
2,6-Dinitrotoluene
Concen: 7.933 ng
RT: 9.93 min Scan# 1333
Delta R.T. 0.22 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01

Tgt Ion:165 Resp: 55506
Ion Ratio Lower Upper
165 100
63 1.2 45.8 68.6#
89 1.5 49.9 74.9#

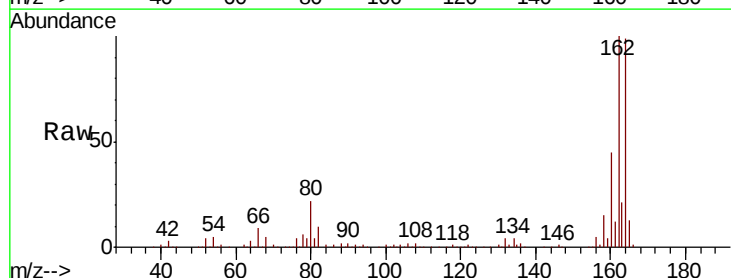

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1



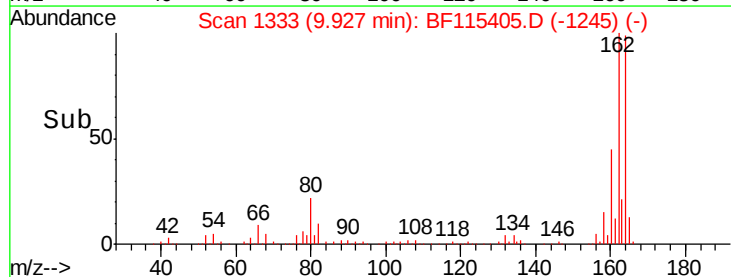
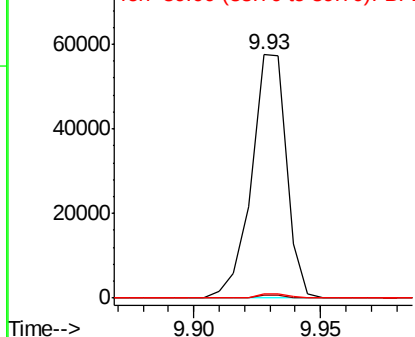


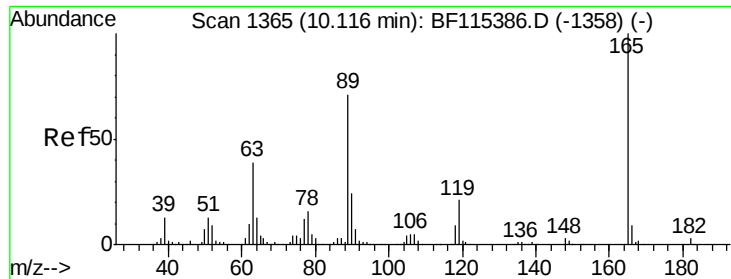

#57
 2,4-Dinitrotoluene
 Concen: 6.243 ng
 RT: 9.93 min Scan# 1333
 Delta R.T. -0.19 min
 Lab File: BF115405.D
 Acq: 8 Jul 2019 15:01




Instrument :
 BNA_E
 ClientSampleId :
 PB121130BL


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.2	31.4	47.0#
89	1.5	57.1	85.7#
182	0.0	2.2	3.2#

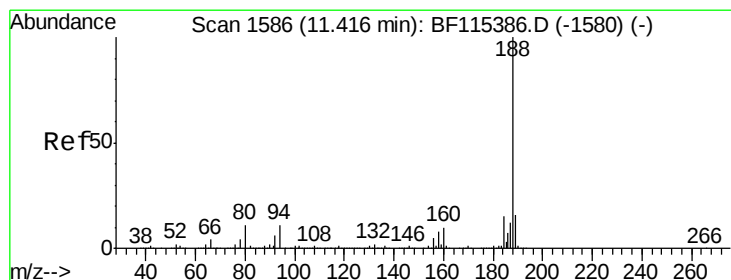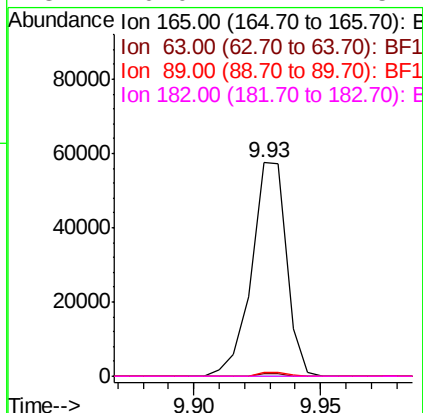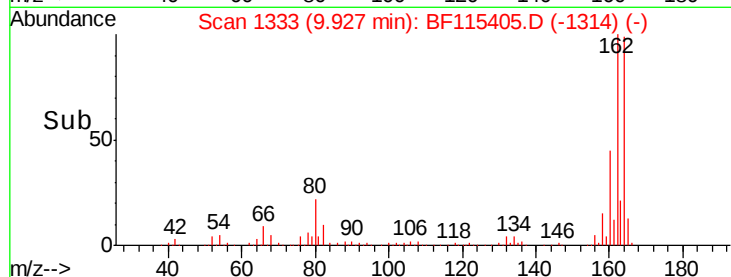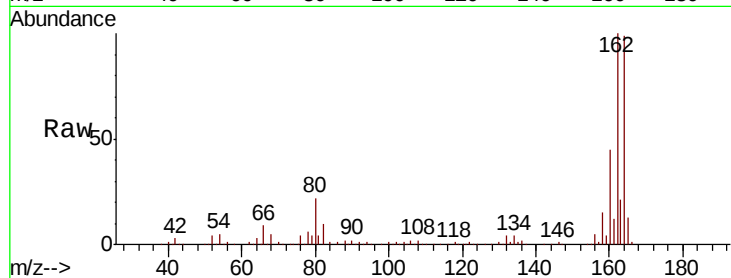

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.42 min Scan# 1586
 Delta R.T. -0.00 min
 Lab File: BF115405.D
 Acq: 8 Jul 2019 15:01

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.8	8.5	12.7
80	10.6	9.1	13.7

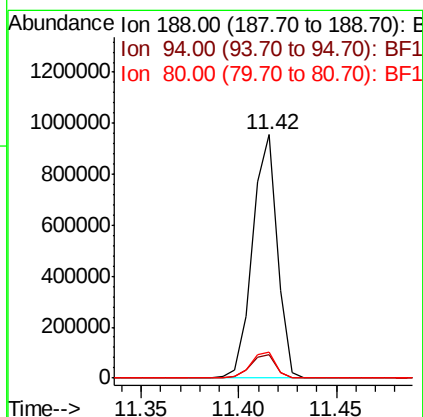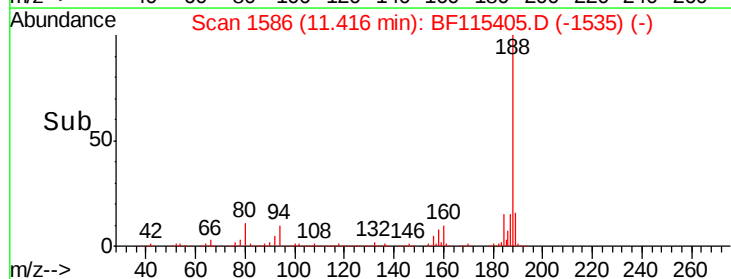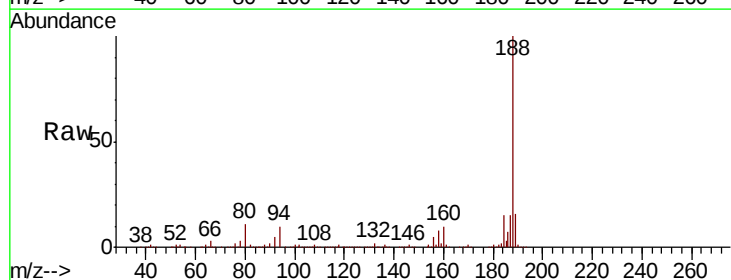


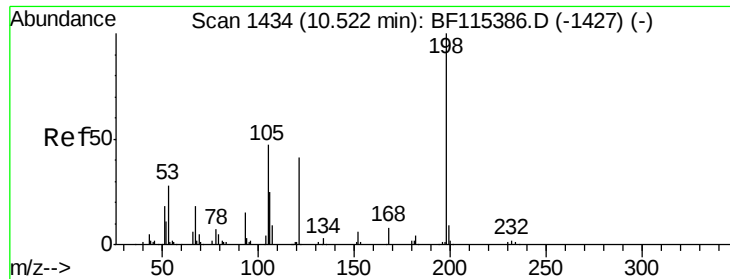




#65
4,6-Dinitro-2-methylphenol
Concen: 8.044 ng
RT: 10.72 min Scan# 1467
Delta R.T. 0.19 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01

Instrument :
BNA_E
ClientSampleId :
PB121130BL

Tot Ion:198 Resp: 1088
Ion Ratio Lower Upper
198 100
51 146.6 25.4 65.4#
105 174.8 27.9 67.9#

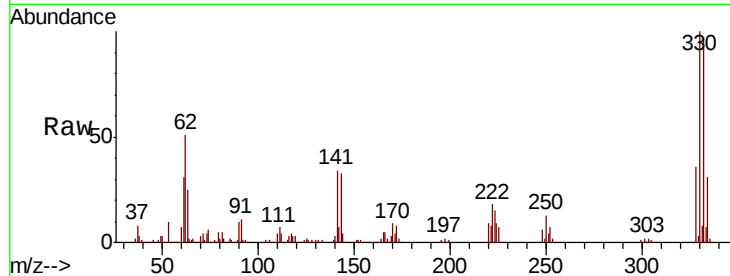


Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF1
Ion 105.00 (104.70 to 105.70): E


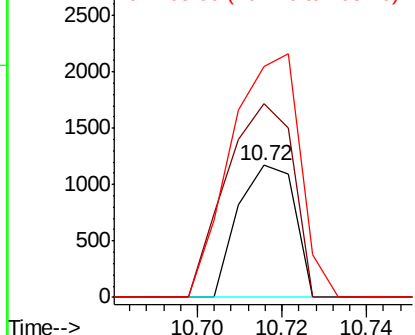



#67
4-Bromophenyl-phenylether
Concen: 3.667 ng
RT: 10.72 min Scan# 1468
Delta R.T. -0.24 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01

Tgt Ion:248 Resp: 34583
Ion Ratio Lower Upper
248 100
250 194.3 77.3 115.9#
141 440.9 58.5 87.7#



Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

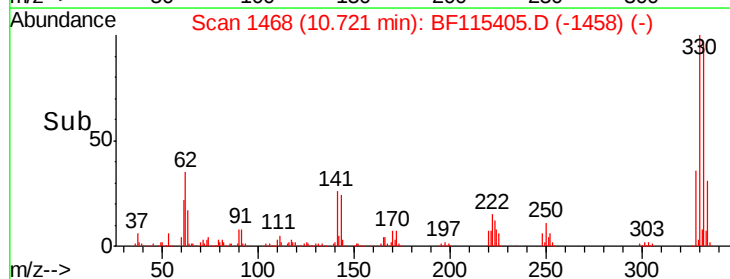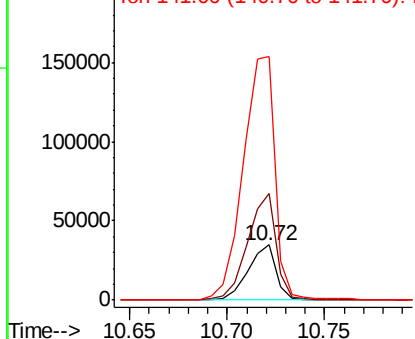



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.06 min Scan# 2035

Delta R.T. -0.01 min

Lab File: BF115405.D

Acq: 8 Jul 2019 15:01

Instrument :

BNA_E

ClientSampleId :

PB121130BL


Tot Ion:240 Resp: 604848

Ion Ratio Lower Upper

240 100

120 12.4 9.1 13.7




236 27.2 22.5 33.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

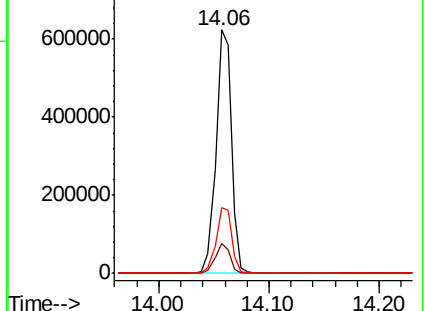

#79

Terphenyl-d14

Concen: 85.559 ng

RT: 13.00 min Scan# 1856

Delta R.T. -0.00 min

Lab File: BF115405.D

Acq: 8 Jul 2019 15:01


Tgt Ion:244 Resp: 2527486

Ion Ratio Lower Upper

244 100

212 7.3 5.7 8.5



122 11.3 9.1 13.7






Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

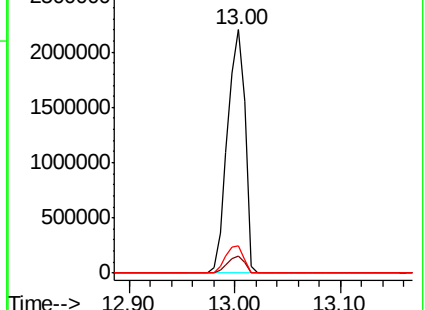

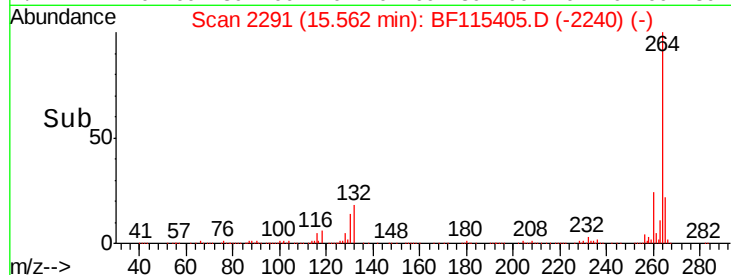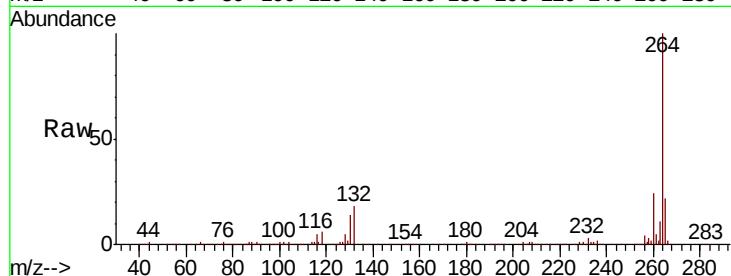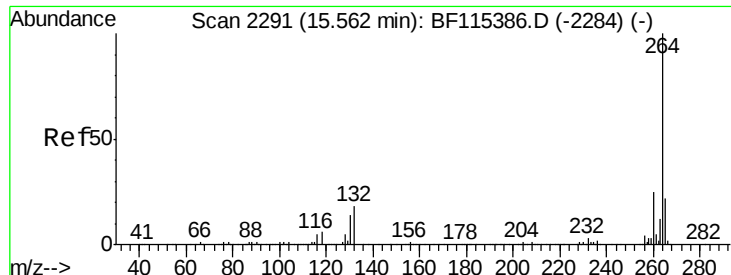

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.56 min Scan# 2291
Delta R.T. -0.00 min
Lab File: BF115405.D
Acq: 8 Jul 2019 15:01

Instrument :
BNA_E
ClientSampleId :
PB121130BL

Tot Ion:	264	Resp:	543523
Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.9	29.9
265	21.7	17.4	26.2

