


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE070819\
 Data File : BE100406.D
 Acq On : 8 Jul 2019 11:22
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 14:06:53 2019

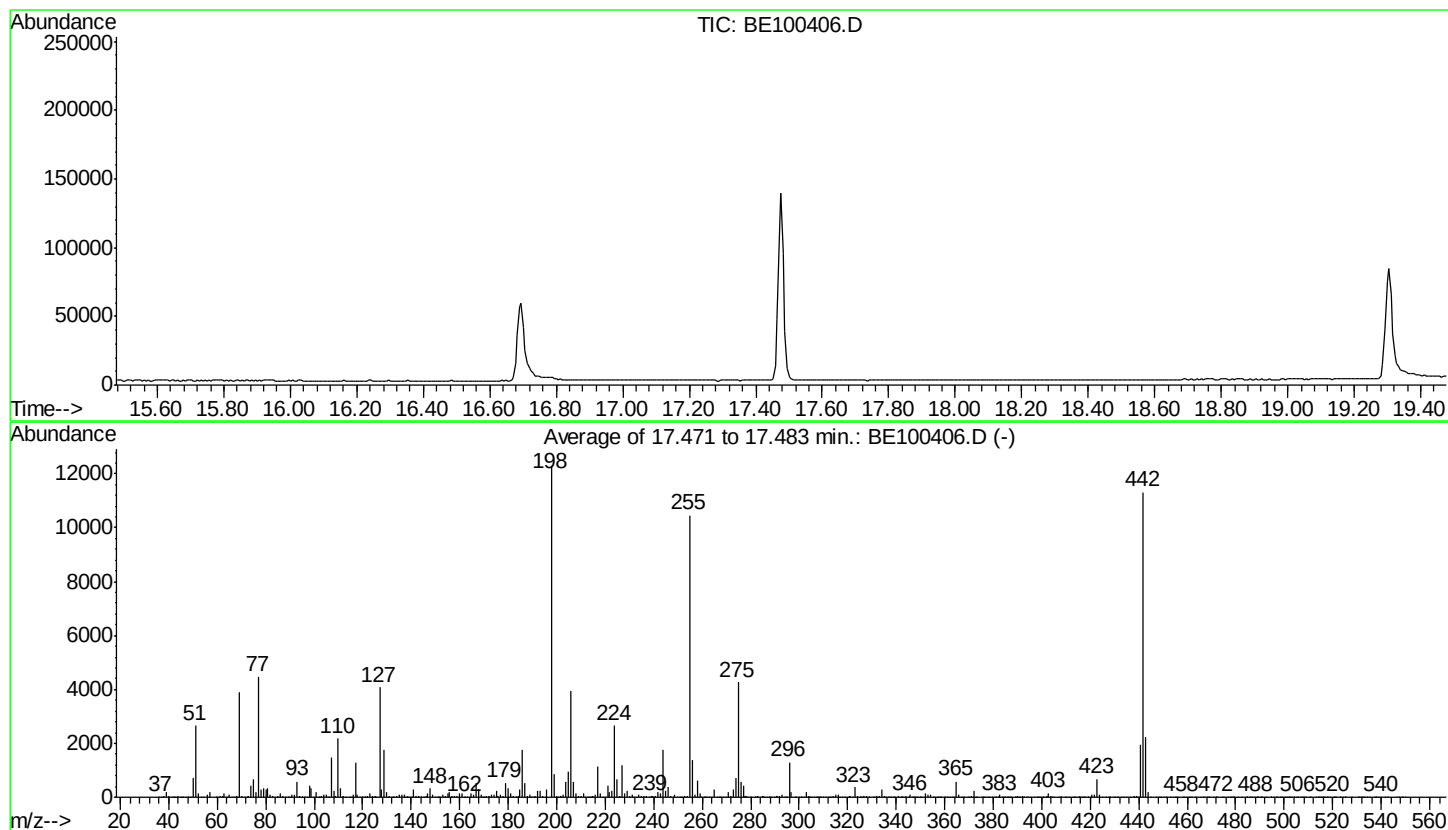

AutoFind: Scans 2533, 2534, 2535; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.5	2645	PASS
68	69	0.00	2	1.8	70	PASS
69	198	0.00	100	31.8	3908	PASS
70	69	0.00	2	0.7	26	PASS
127	198	10	80	33.0	4063	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12304	PASS
199	198	5	9	6.8	837	PASS
275	198	10	60	34.6	4255	PASS
365	198	1	100	4.8	595	PASS
441	198	0.01	100	15.8	1948	PASS
442	198	50	100	92.0	11318	PASS
443	442	15	24	19.9	2257	PASS