


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE072219\
 Data File : BE100476.D
 Acq On : 22 Jul 2019 11:23
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 23 08:06:59 2019

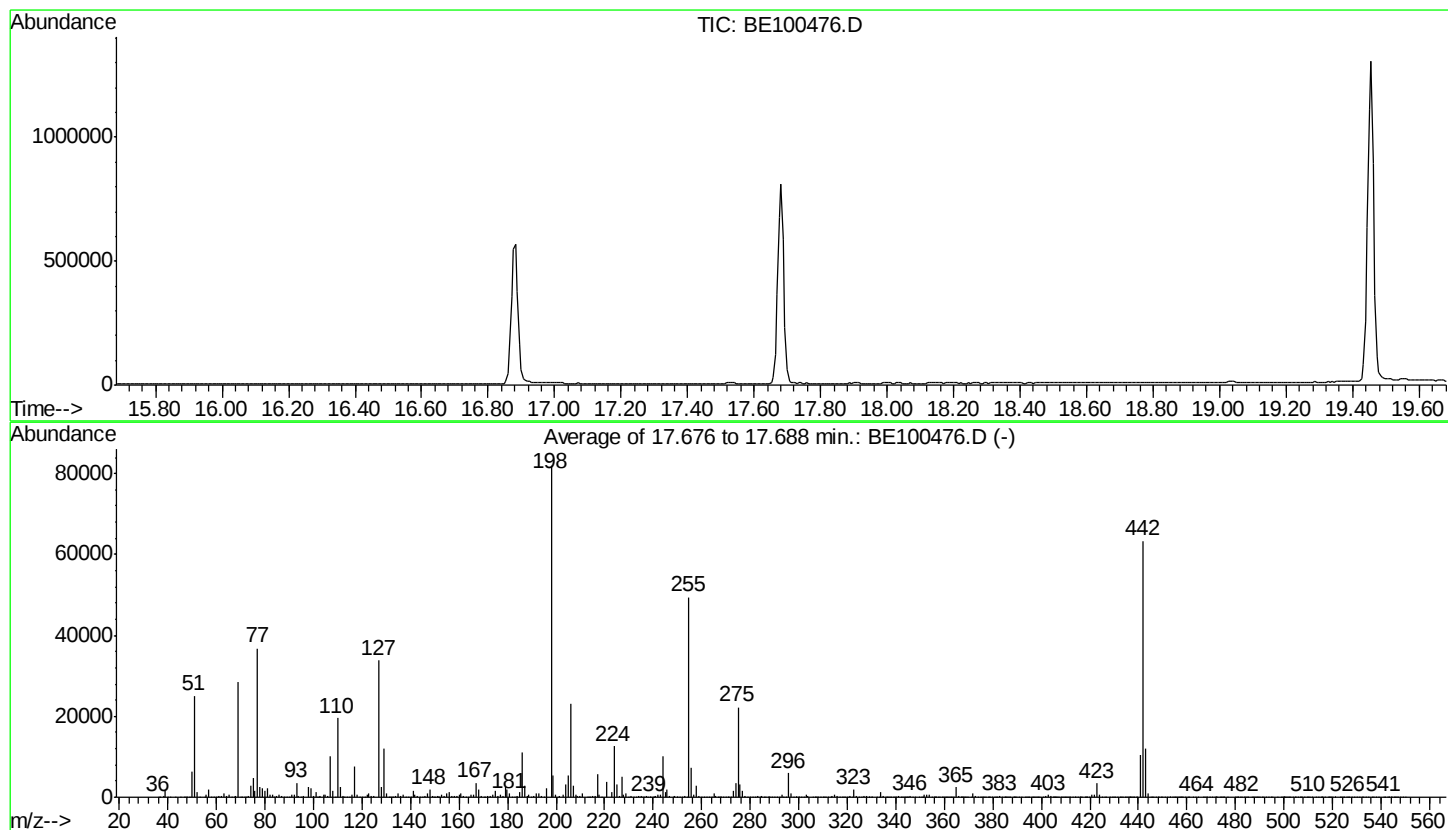

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.7	25151	PASS
68	69	0.00	2	1.6	442	PASS
69	198	0.00	100	34.7	28420	PASS
70	69	0.00	2	0.4	124	PASS
127	198	10	80	41.3	33859	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81972	PASS
199	198	5	9	6.7	5475	PASS
275	198	10	60	27.0	22157	PASS
365	198	1	100	3.1	2519	PASS
441	198	0.01	100	12.7	10416	PASS
442	198	50	100	77.3	63357	PASS
443	442	15	24	19.1	12091	PASS