


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE072319\
Data File : BE100490.D
Acq On : 23 Jul 2019 7:51
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072219.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 23 08:06:59 2019

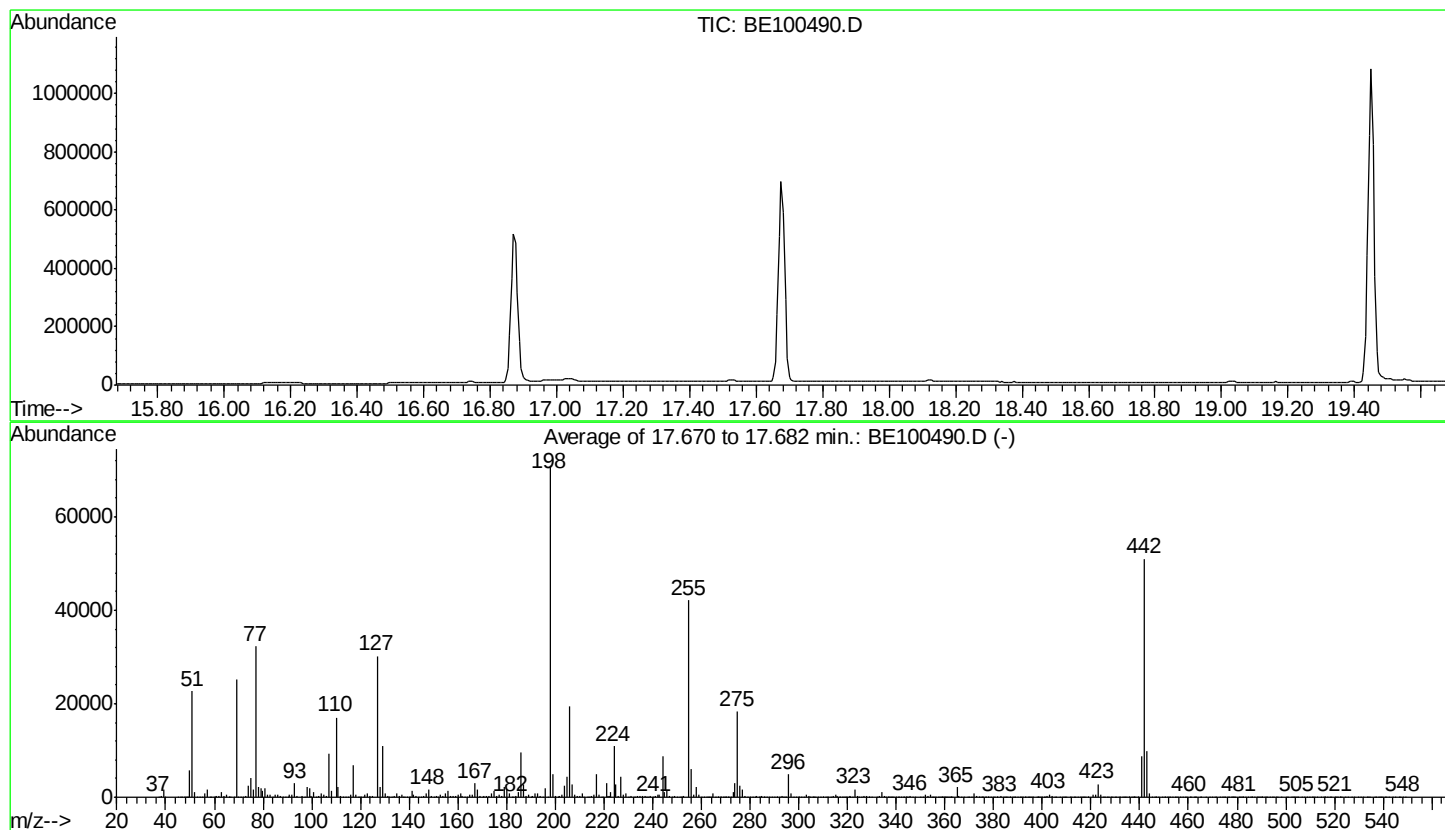

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	22664	PASS
68	69	0.00	2	0.3	86	PASS
69	198	0.00	100	35.4	25086	PASS
70	69	0.00	2	0.2	39	PASS
127	198	10	80	42.5	30140	PASS
197	198	0.00	2	0.1	106	PASS
198	198	100	100	100.0	70933	PASS
199	198	5	9	6.9	4883	PASS
275	198	10	60	25.8	18276	PASS
365	198	1	100	2.9	2072	PASS
441	198	0.01	100	12.5	8833	PASS
442	198	50	100	71.9	50990	PASS
443	442	15	24	19.5	9934	PASS