


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE113018\
 Data File : BE098282.D
 Acq On : 30 Nov 2018 9:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE112918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 29 13:50:43 2018

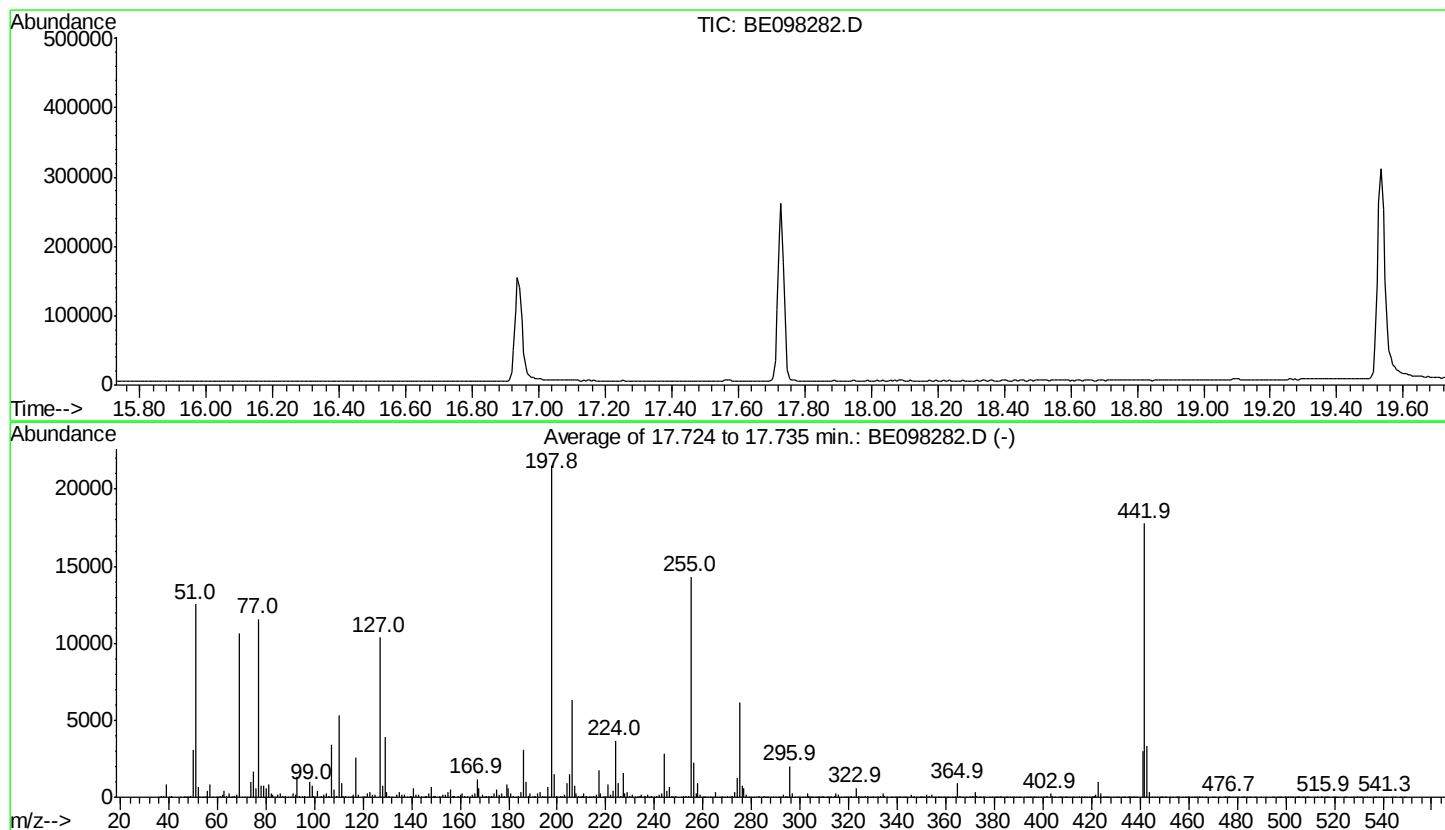

AutoFind: Scans 2576, 2577, 2578; Background Corrected with Scan 2569

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.2	12524	PASS
68	69	0.00	2	1.4	153	PASS
69	198	0.00	100	49.6	10674	PASS
70	69	0.00	2	0.4	40	PASS
127	198	10	80	48.2	10371	PASS
197	198	0.00	2	0.2	42	PASS
198	198	100	100	100.0	21531	PASS
199	198	5	9	7.0	1504	PASS
275	198	10	60	28.6	6148	PASS
365	198	1	100	4.1	885	PASS
441	198	0.01	100	13.9	2991	PASS
442	198	50	100	82.6	17787	PASS
443	442	15	24	18.5	3290	PASS