


Data Path : Z:\HPCHEM1\BNA_E\Data\BE010215\
 Data File : BE089301.D
 Acq On : 2 Jan 2015 9:58
 Operator : TP/IZ
 Sample : DFTPP34
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP34

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 02 10:52:56 2015

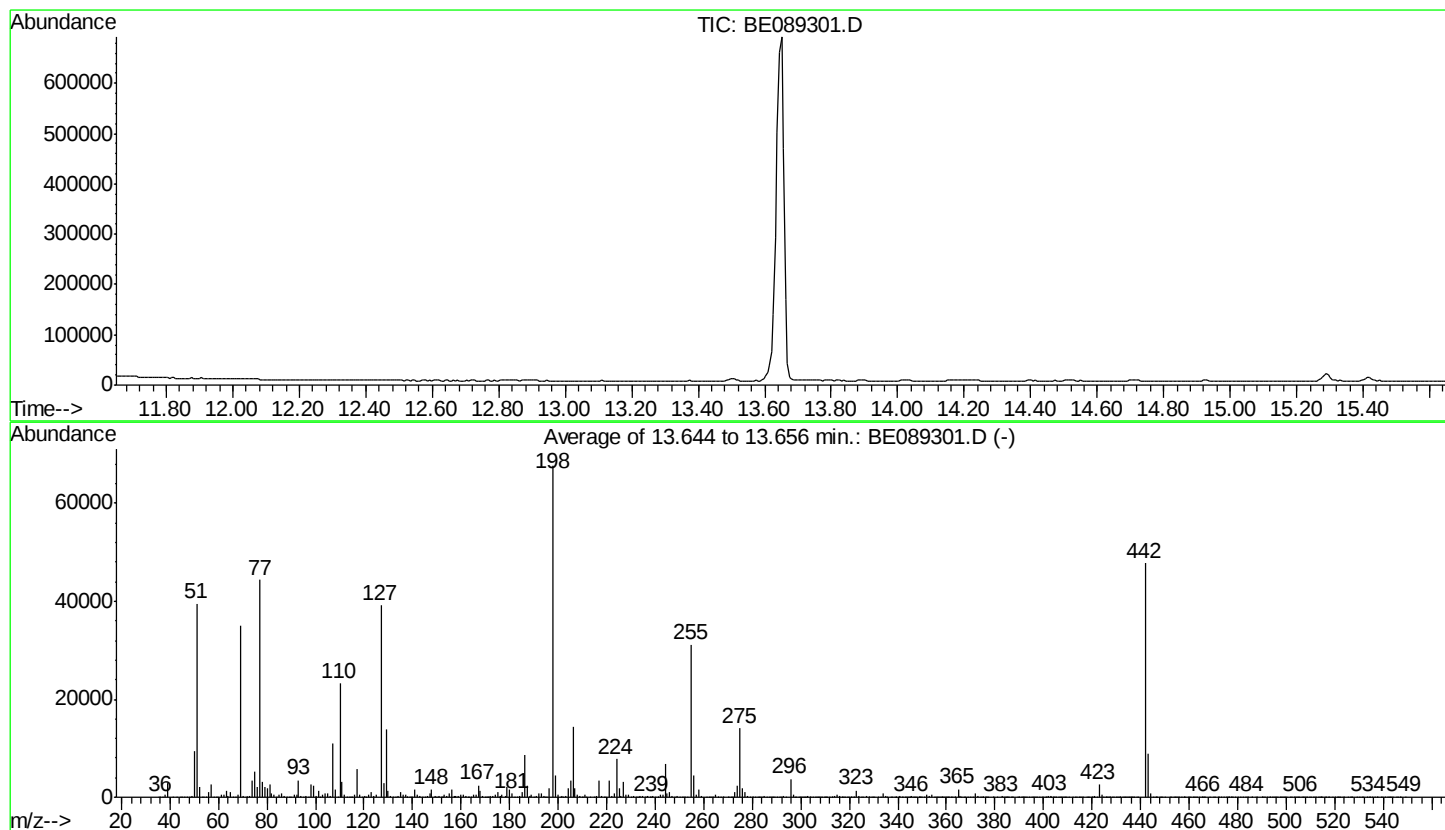

AutoFind: Scans 2086, 2087, 2088; Background Corrected with Scan 2072

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.5	39594	PASS
68	69	0.00	2	1.3	468	PASS
69	198	0.00	100	51.6	34910	PASS
70	69	0.00	2	0.5	170	PASS
127	198	10	80	57.8	39104	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	67703	PASS
199	198	5	9	6.4	4340	PASS
275	198	10	60	20.7	14004	PASS
365	198	1	100	2.5	1706	PASS
441	443	0.01	100	0.0	0	FAIL *
442	198	50	100	70.5	47744	PASS
443	442	15	24	18.6	8900	PASS