

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010215\
 Data File : BE089308.D
 Acq On : 2 Jan 2015 16:29
 Operator : TP/IZ
 Sample : PB81158BL
 Misc : SBLK82
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK82

Quant Time: Jan 05 09:08:46 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 02 22:03:42 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1832	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	7440	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.65	164	3770	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	5712	0.40	ng/ul	0.00
18) Chrysene-d12	18.06	240	3585	0.40	ng/ul	0.00
22) Perylene-d12	21.11	264	2771	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.18	96	5228	1.90	ng/uL	0.02
6) 2-Methylnaphthalene-d10	0.00	152	0	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
17) Fluoranthene	14.96	202	2184	0.04	ng/ul	Qvalue 76
19) Pyrene	15.41	202	2391	0.05	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010215\
Data File : BE089308.D
Acq On : 2 Jan 2015 16:29
Operator : TP/IZ
Sample : PB81158BL
Misc : SBLK82
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK82

Quant Time: Jan 05 09:08:46 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 02 22:03:42 2015
Response via : Initial Calibration




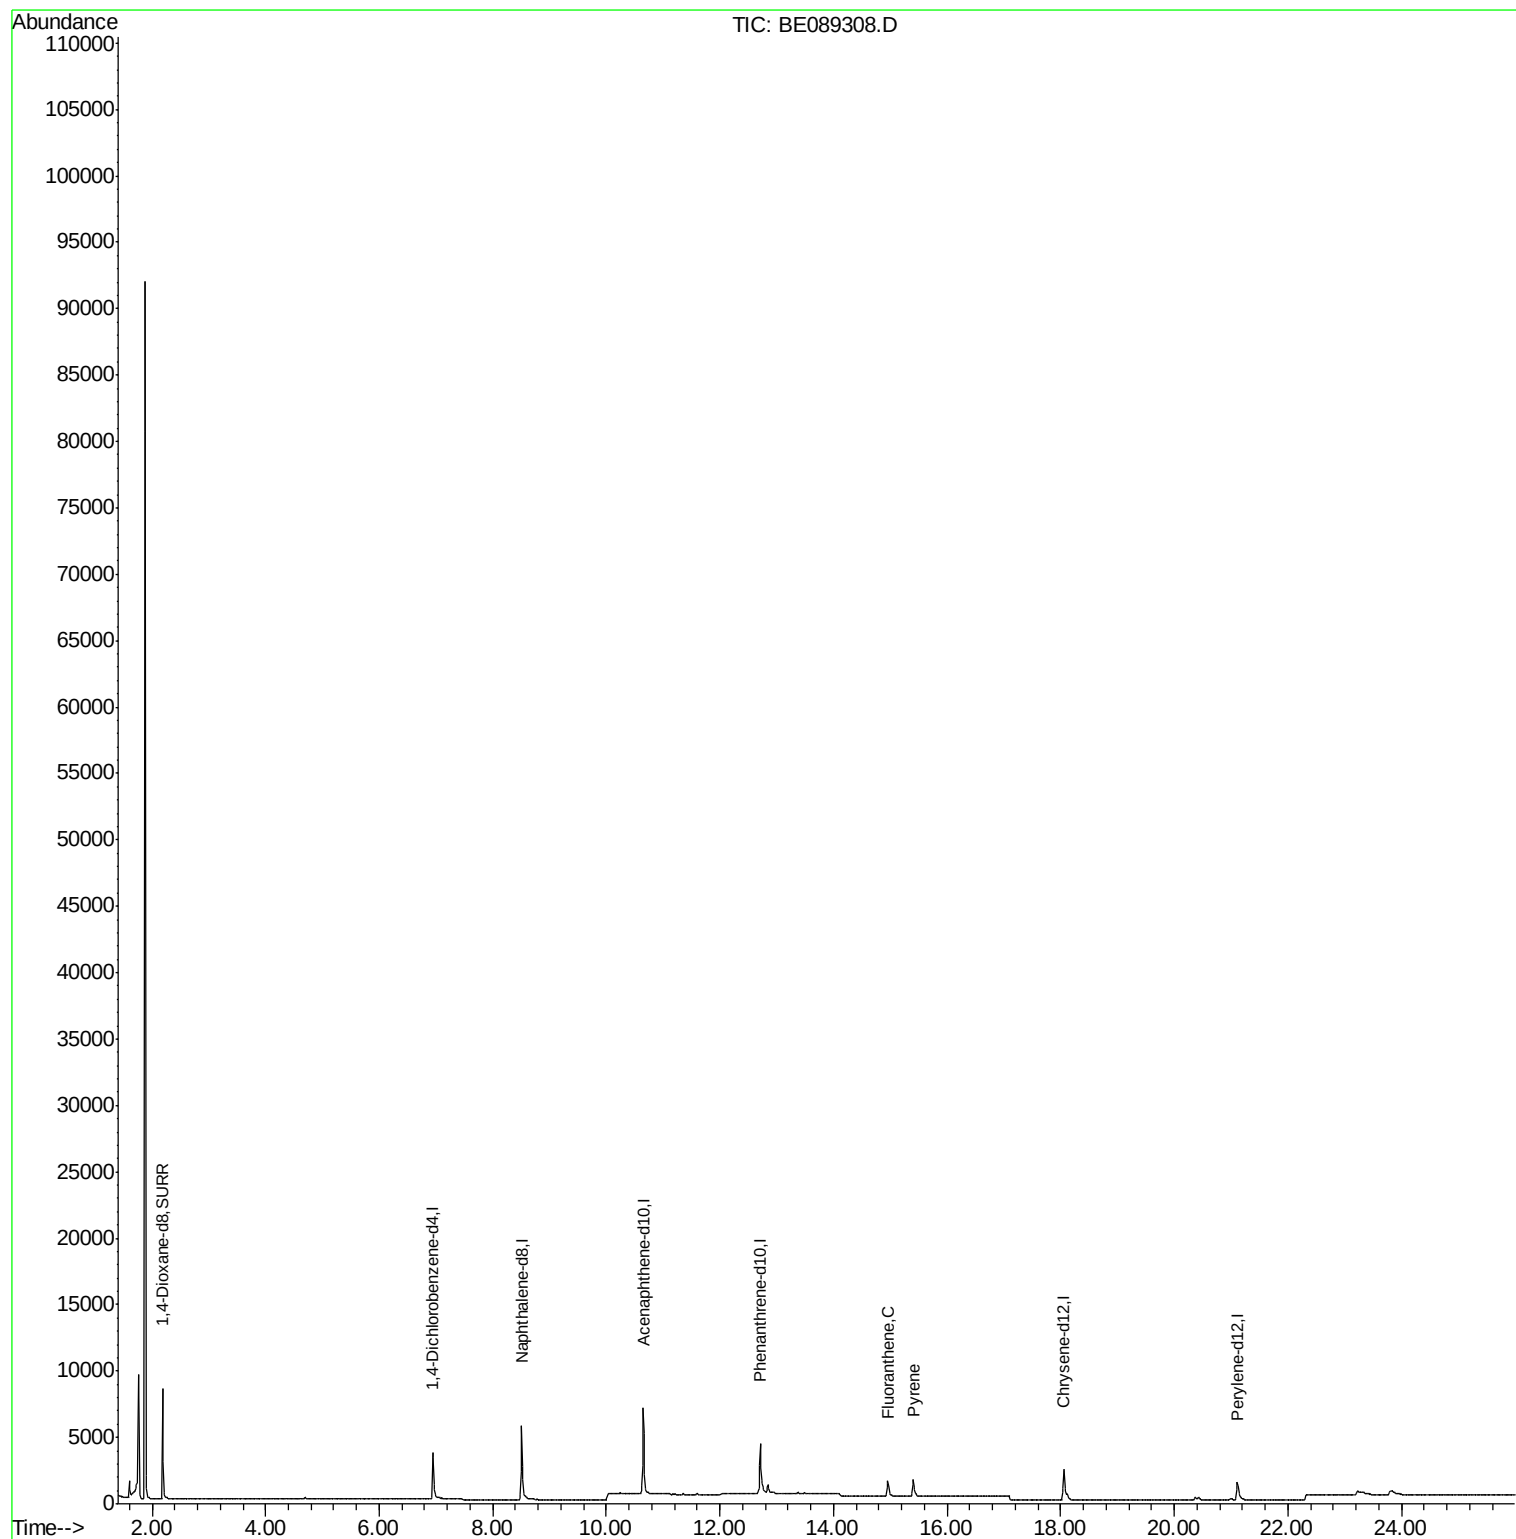


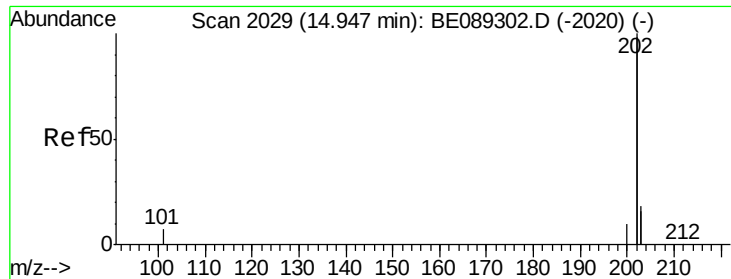

#17
Fluoranthene
 Concen: 0.04 ng/ul
 RT: 14.96 min Scan# 2031
 Delta R.T. 0.01 min
 Lab File: BE089308.D
 Acq: 2 Jan 2015 16:29

Instrument :
 BNA_E
 ClientSampled :
 SBLK82

Tgt Ion:202 Resp: 2184
 Ion Ratio Lower Upper
 202 100
 101 7.3 0.0 24.6
 203 30.3 0.0 37.8

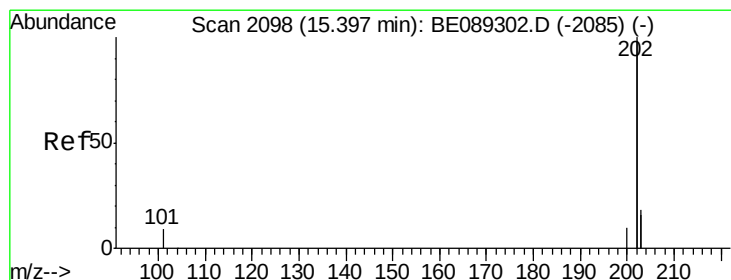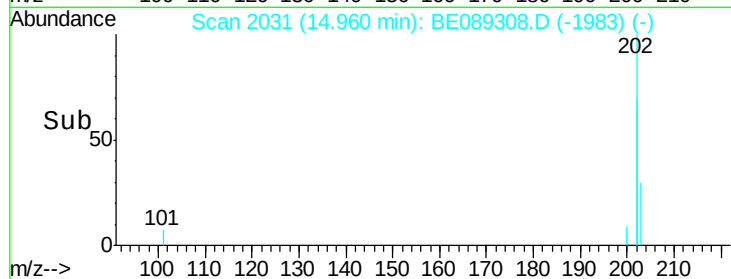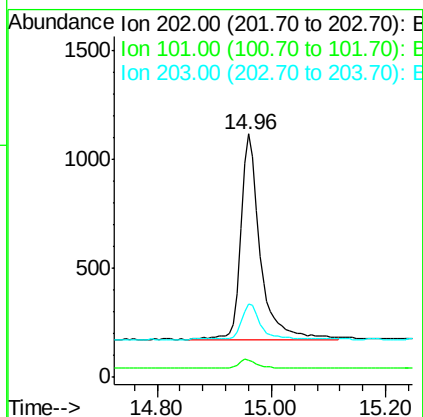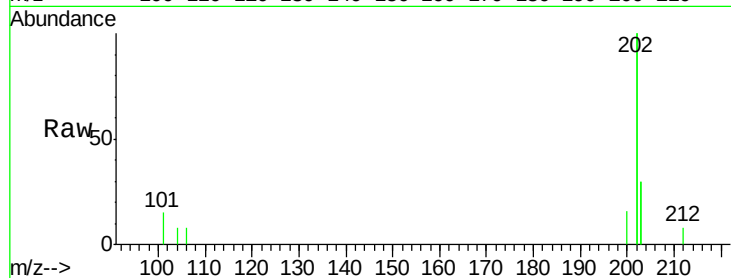

#19
Pyrene
 Concen: 0.05 ng/ul
 RT: 15.41 min Scan# 2100
 Delta R.T. 0.01 min
 Lab File: BE089308.D
 Acq: 2 Jan 2015 16:29

Tgt Ion:202 Resp: 2391
 Ion Ratio Lower Upper
 202 100
 200 8.0 4.2 6.4#
 203 30.8 14.4 21.6#

