


Data Path : Z:\HPCHEM1\BNA_E\Data\BE010515\
Data File : BE089310.D
Acq On : 5 Jan 2015 10:27
Operator : TP/IZ
Sample : DFTPP35
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP35

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 02 10:52:56 2015

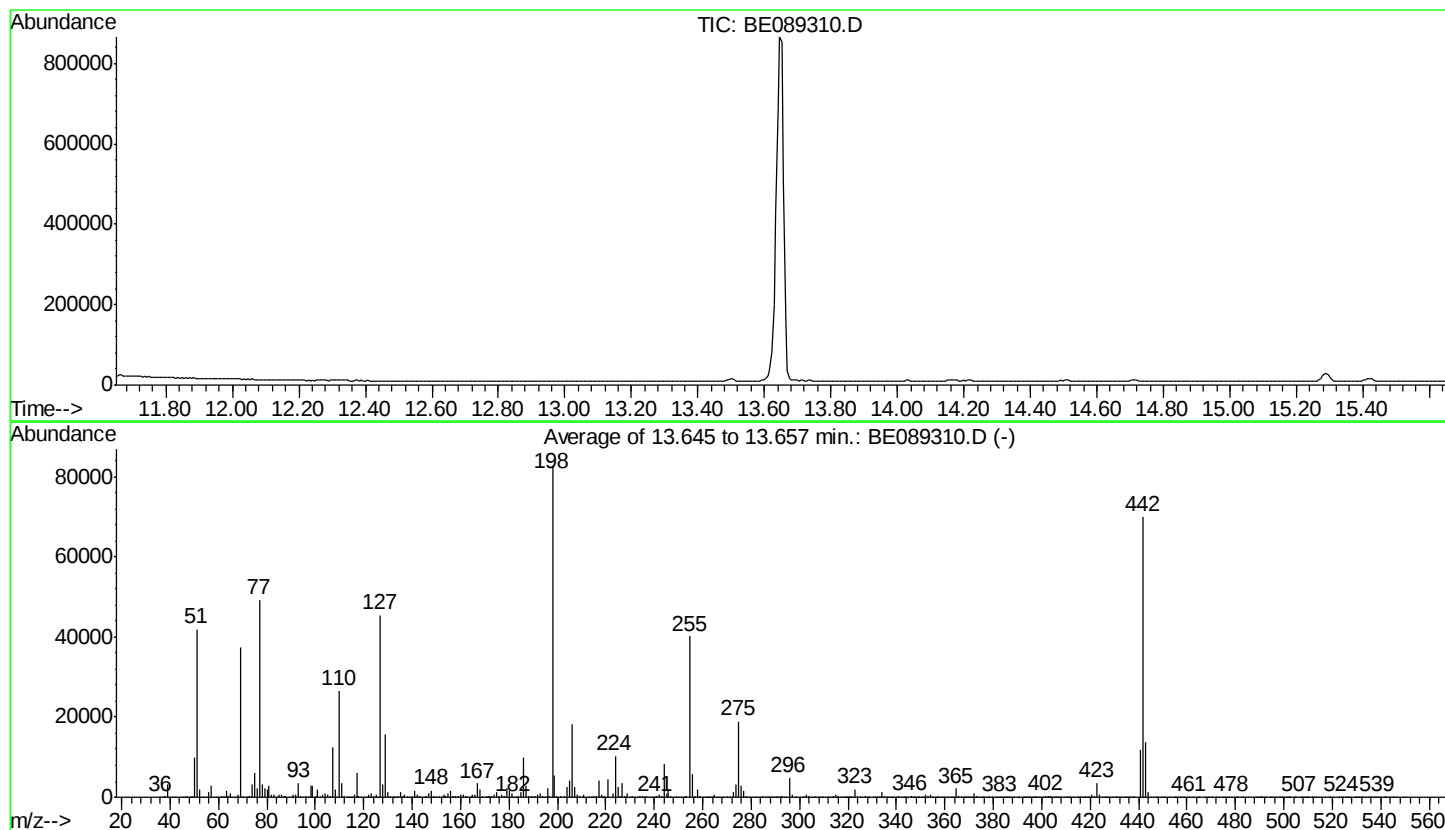

AutoFind: Scans 2086, 2087, 2088; Background Corrected with Scan 2068

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	41943	PASS
68	69	0.00	2	1.4	530	PASS
69	198	0.00	100	45.2	37400	PASS
70	69	0.00	2	0.4	154	PASS
127	198	10	80	54.9	45455	PASS
197	198	0.00	1	0.4	342	PASS
198	198	100	100	100.0	82769	PASS
199	198	5	9	6.5	5371	PASS
275	198	10	60	23.0	19021	PASS
365	198	1	100	2.6	2160	PASS
441	443	0.01	100	87.9	11968	PASS
442	198	50	100	84.7	70068	PASS
443	442	15	24	19.4	13610	PASS