


Data Path : Z:\HPCHEM1\BNA_E\Data\BE010515\
 Data File : BE089318.D
 Acq On : 5 Jan 2015 17:34
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 06 00:09:35 2015

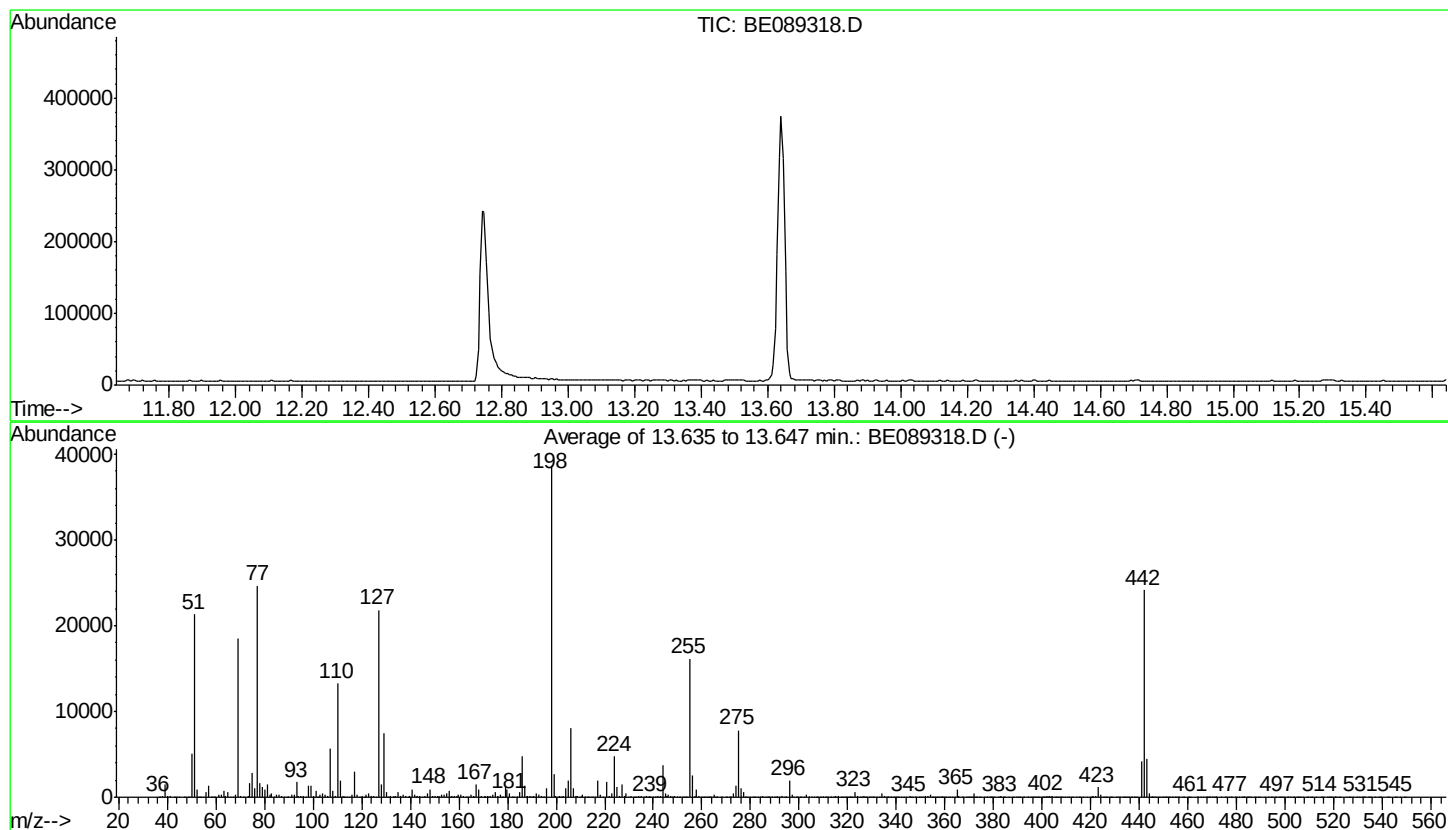

AutoFind: Scans 2084, 2085, 2086; Background Corrected with Scan 2072

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.2	21340	PASS
68	69	0.00	2	1.4	264	PASS
69	198	0.00	100	47.7	18450	PASS
70	69	0.00	2	0.6	113	PASS
127	198	10	80	56.4	21796	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	38669	PASS
199	198	5	9	6.8	2631	PASS
275	198	10	60	20.2	7827	PASS
365	198	1	100	2.2	855	PASS
441	443	0.01	100	92.6	4203	PASS
442	198	50	100	62.4	24146	PASS
443	442	15	24	18.8	4540	PASS