

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010515\
 Data File : BE089312.D
 Acq On : 5 Jan 2015 14:11
 Operator : TP/IZ
 Sample : F5245-10RX
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Y9RA4

Quant Time: Jan 06 12:56:45 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 06 00:09:29 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1448	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	5835	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.65	164	3013	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	4537	0.40	ng/ul	0.01
18) Chrysene-d12	18.06	240	2549	0.40	ng/ul	0.00
22) Perylene-d12	21.11	264	2000	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.20	96	578	0.27	ng/uL	0.03
6) 2-Methylnaphthalene-d10	0.00	152	0	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
17) Fluoranthene	14.95	202	1558	0.04	ng/ul	Qvalue 73
19) Pyrene	15.40	202	1658	0.05	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010515\
Data File : BE089312.D
Acq On : 5 Jan 2015 14:11
Operator : TP/IZ
Sample : F5245-10RX
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Y9RA4

Quant Time: Jan 06 12:56:45 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 06 00:09:29 2015
Response via : Initial Calibration




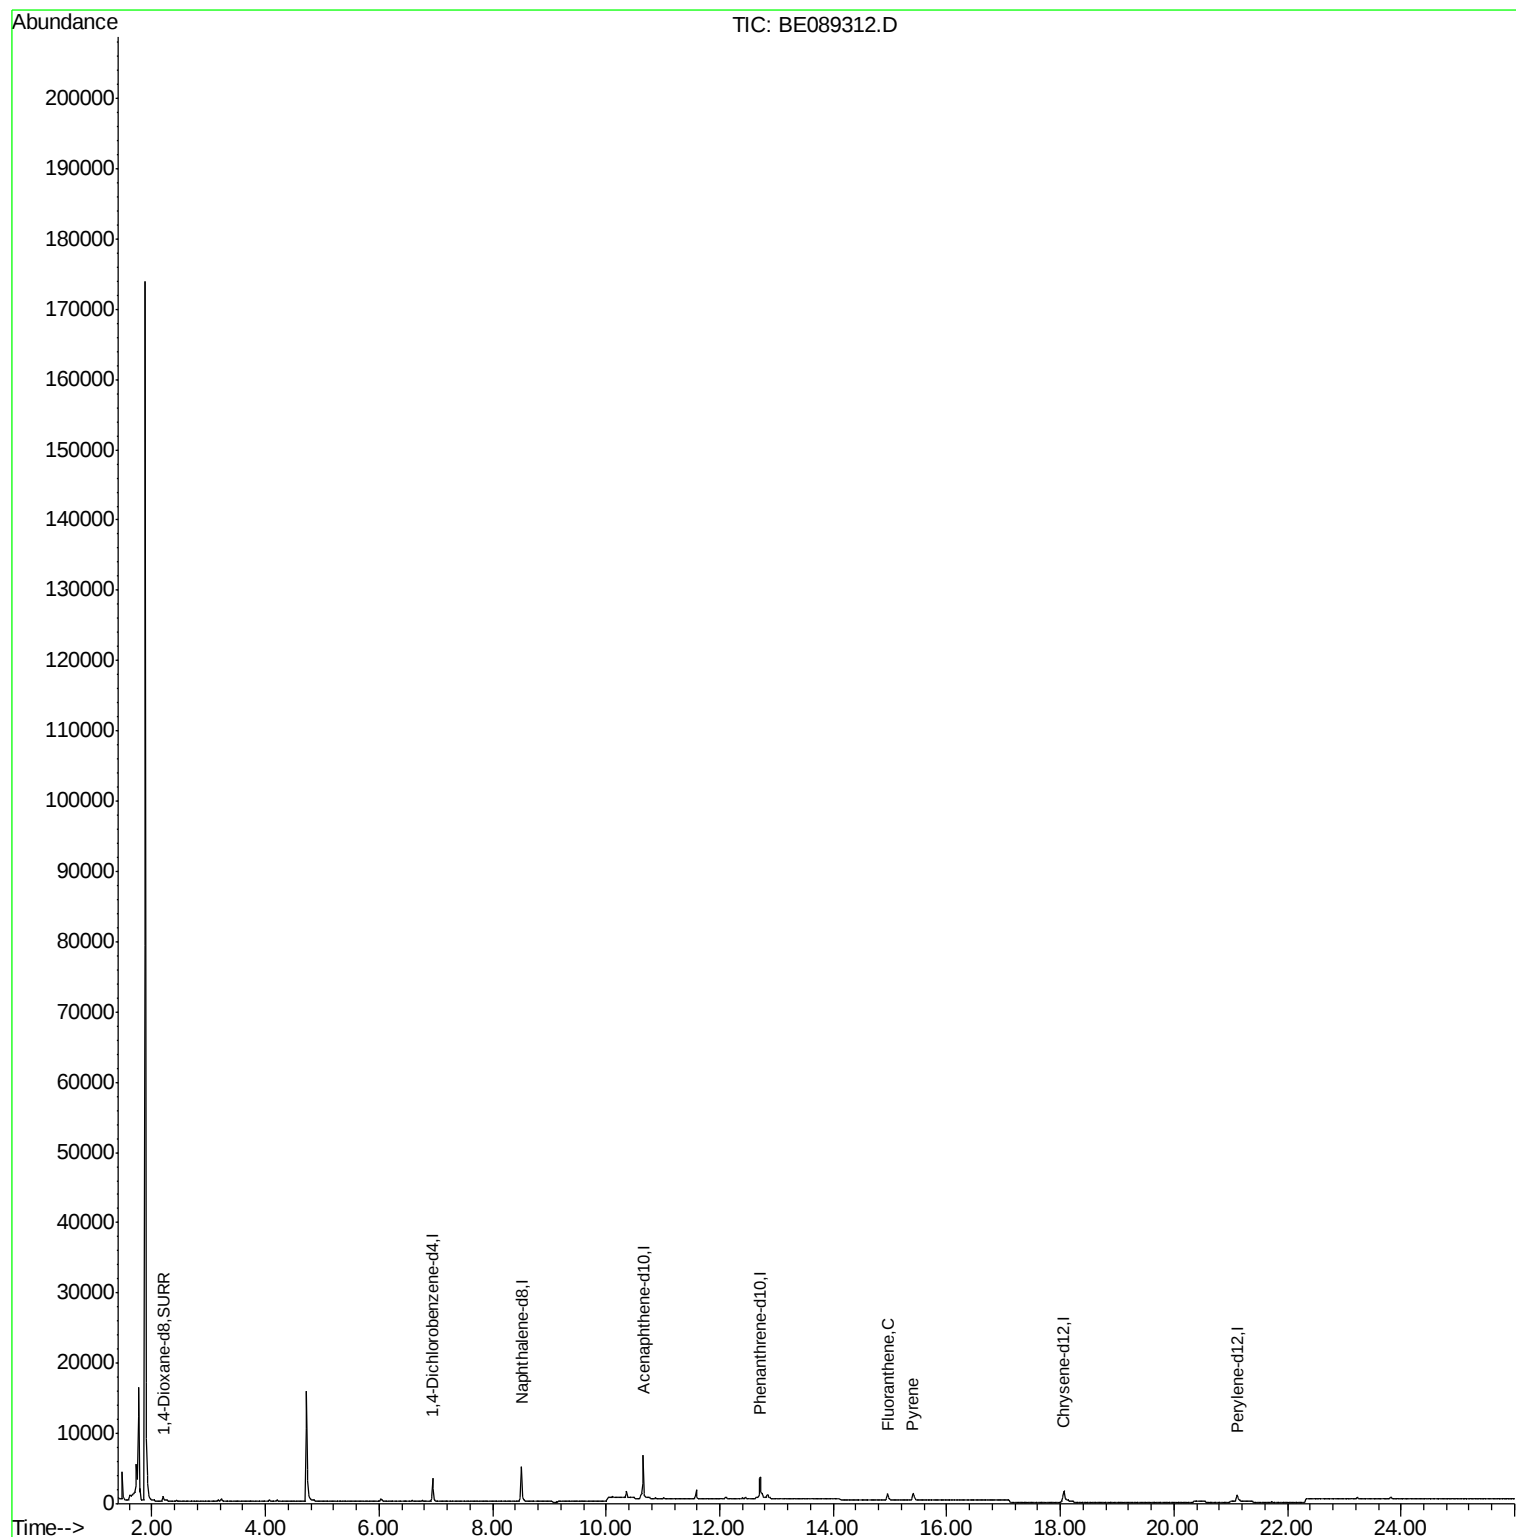


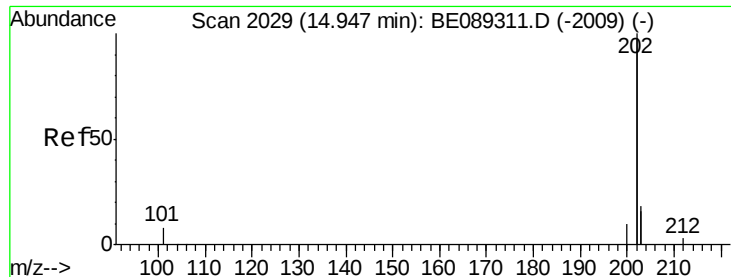

#17
Fluoranthene
 Concen: 0.04 ng/ul
 RT: 14.95 min Scan# 2029
 Delta R.T. 0.01 min
 Lab File: BE089312.D
 Acq: 5 Jan 2015 14:11

Instrument :
 BNA_E
 ClientSampleId :
 Y9RA4

Tgt Ion:202 Resp: 1558
 Ion Ratio Lower Upper
 202 100
 101 7.9 0.0 24.6
 203 31.9 0.0 37.8

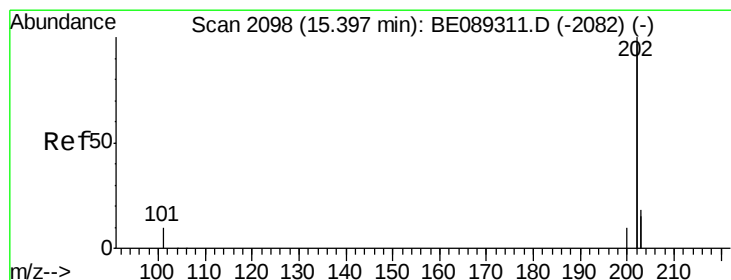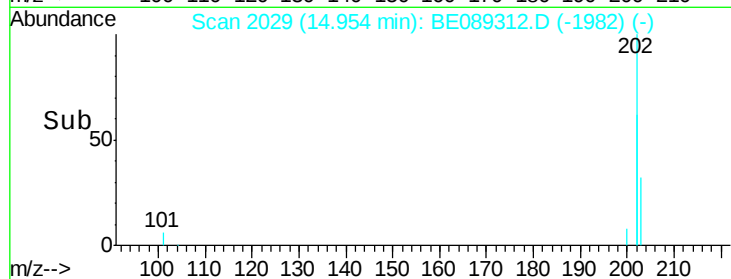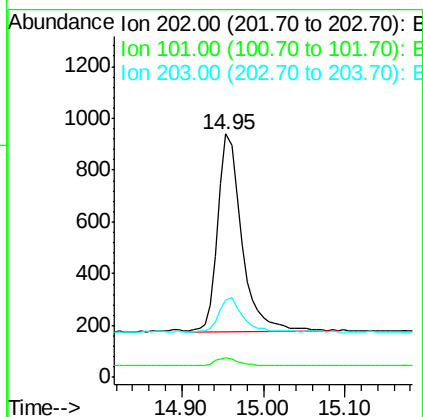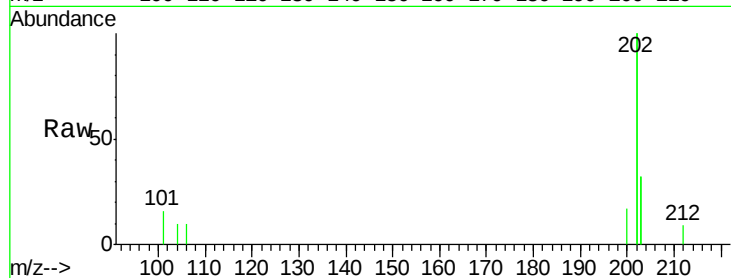

#19
Pyrene
 Concen: 0.05 ng/ul
 RT: 15.40 min Scan# 2098
 Delta R.T. 0.01 min
 Lab File: BE089312.D
 Acq: 5 Jan 2015 14:11

Tgt Ion:202 Resp: 1658
 Ion Ratio Lower Upper
 202 100
 200 9.0 4.2 6.4#
 203 33.3 14.4 21.6#

