


Data Path : Z:\HPCHEM1\BNA E\Data\BE010617\
Data File : BE092629.D
Acq On : 6 Jan 2017 13:08
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121916.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Dec 19 16:16:32 2016

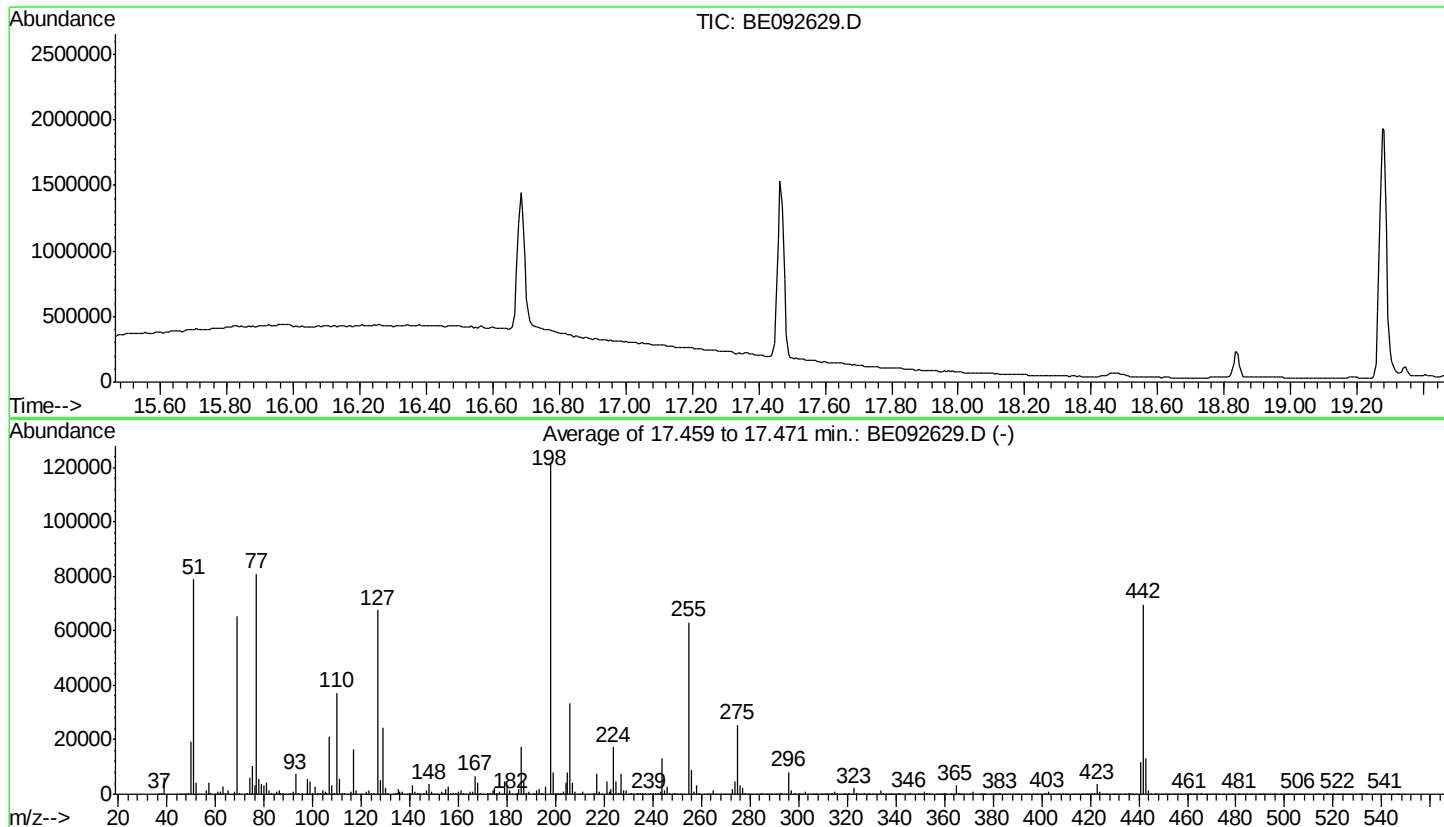

AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2523

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.7	78756	PASS
68	69	0.00	2	1.3	866	PASS
69	198	0.00	100	53.5	65152	PASS
70	69	0.00	2	0.6	419	PASS
127	198	10	80	55.4	67442	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121706	PASS
199	198	5	9	6.5	7865	PASS
275	198	10	60	20.9	25464	PASS
365	198	1	100	2.6	3177	PASS
441	442	0.01	24	17.2	11953	PASS
442	198	50	100	57.2	69563	PASS
443	442	15	24	19.1	13281	PASS