


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010715\
 Data File : BE089349.D
 Acq On : 8 Jan 2015 3:06
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BASE-BE010715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 08 06:03:23 2015

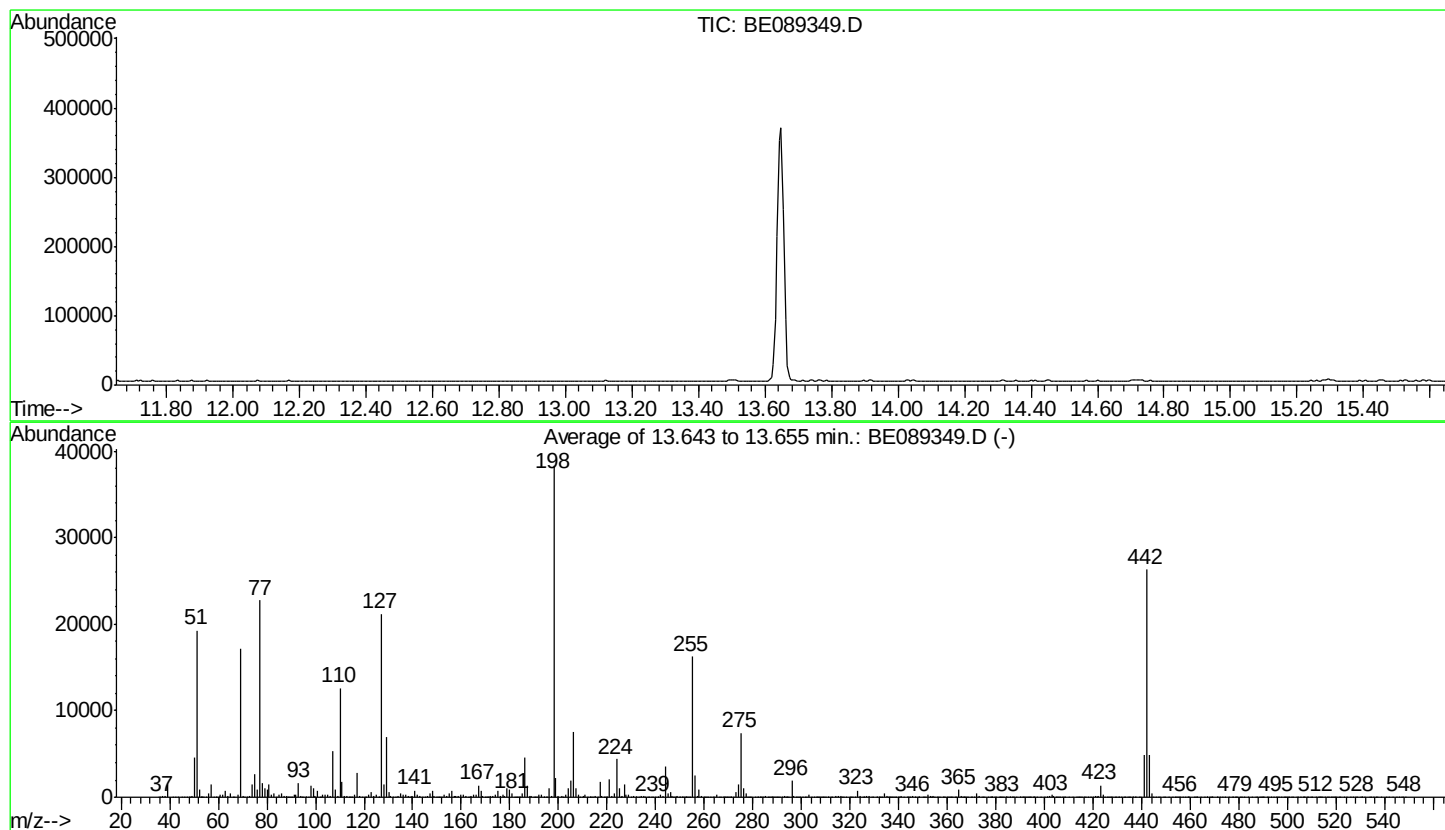

AutoFind: Scans 2086, 2087, 2088; Background Corrected with Scan 2076

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	19279	PASS
68	69	0.00	2	1.4	243	PASS
69	198	0.00	100	44.8	17189	PASS
70	69	0.00	2	0.6	96	PASS
127	198	10	80	55.4	21226	PASS
197	198	0.00	2	0.2	87	PASS
198	198	100	100	100.0	38330	PASS
199	198	5	9	6.0	2283	PASS
275	198	10	60	19.5	7473	PASS
365	198	1	100	2.3	885	PASS
441	442	0.01	24	18.4	4839	PASS
442	198	50	100	68.7	26329	PASS
443	442	15	24	18.8	4958	PASS