


Data Path : Z:\HPCHEM1\BNA_E\Data\BE010715\
 Data File : Be089325.d
 Acq On : 7 Jan 2015 9:54
 Operator : TP/IZ
 Sample : DFTPP36
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP36

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 02 10:52:56 2015

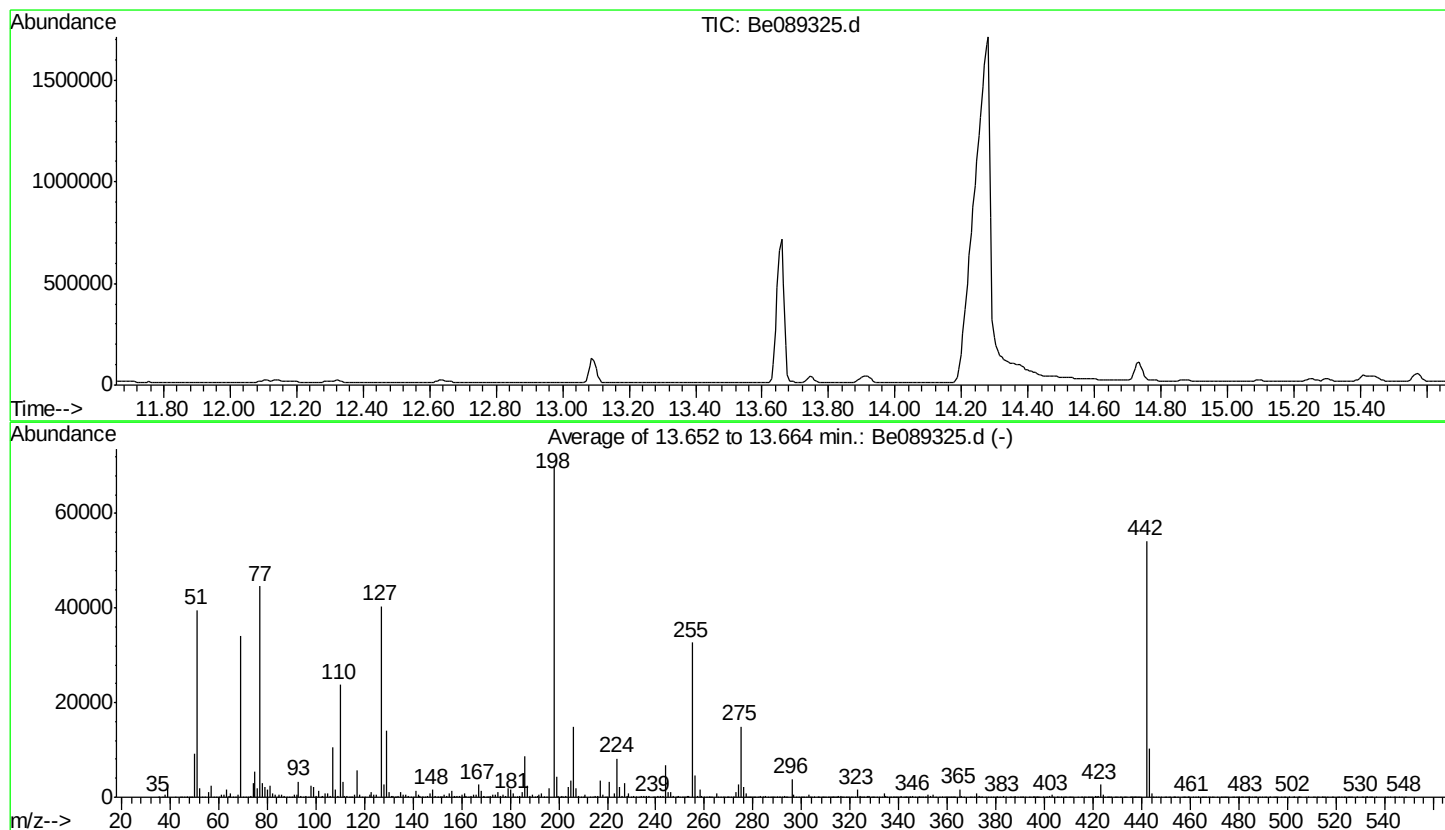

AutoFind: Scans 2087, 2088, 2089; Background Corrected with Scan 2078

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.4	39552	PASS
68	69	0.00	2	1.2	421	PASS
69	198	0.00	100	48.5	34046	PASS
70	69	0.00	2	0.4	124	PASS
127	198	10	80	57.6	40390	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	70136	PASS
199	198	5	9	6.3	4445	PASS
275	198	10	60	21.3	14908	PASS
365	198	1	100	2.4	1660	PASS
441	443	0.01	100	0.0	0	FAIL *
442	198	50	100	77.3	54197	PASS
443	442	15	24	19.0	10295	PASS