

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010715\
 Data File : BE089332.D
 Acq On : 7 Jan 2015 14:37
 Operator : TP/IZ
 Sample : F5245-19
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Y9RB5

Quant Time: Jan 08 13:05:01 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 02 10:52:56 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1269	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	5037	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.66	164	2588	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	3940	0.40	ng/ul	0.00
18) Chrysene-d12	18.07	240	2782	0.40	ng/ul	0.00
22) Perylene-d12	21.12	264	2379	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.12	96	465	0.24	ng/uL	-0.03
6) 2-Methylnaphthalene-d10	0.00	152	0	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
17) Fluoranthene	14.95	202	1299	0.03	ng/ul	Qvalue 69
19) Pyrene	15.40	202	1371	0.04	ng/ul#	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010715\
Data File : BE089332.D
Acq On : 7 Jan 2015 14:37
Operator : TP/IZ
Sample : F5245-19
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Y9RB5

Quant Time: Jan 08 13:05:01 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 02 10:52:56 2015
Response via : Initial Calibration




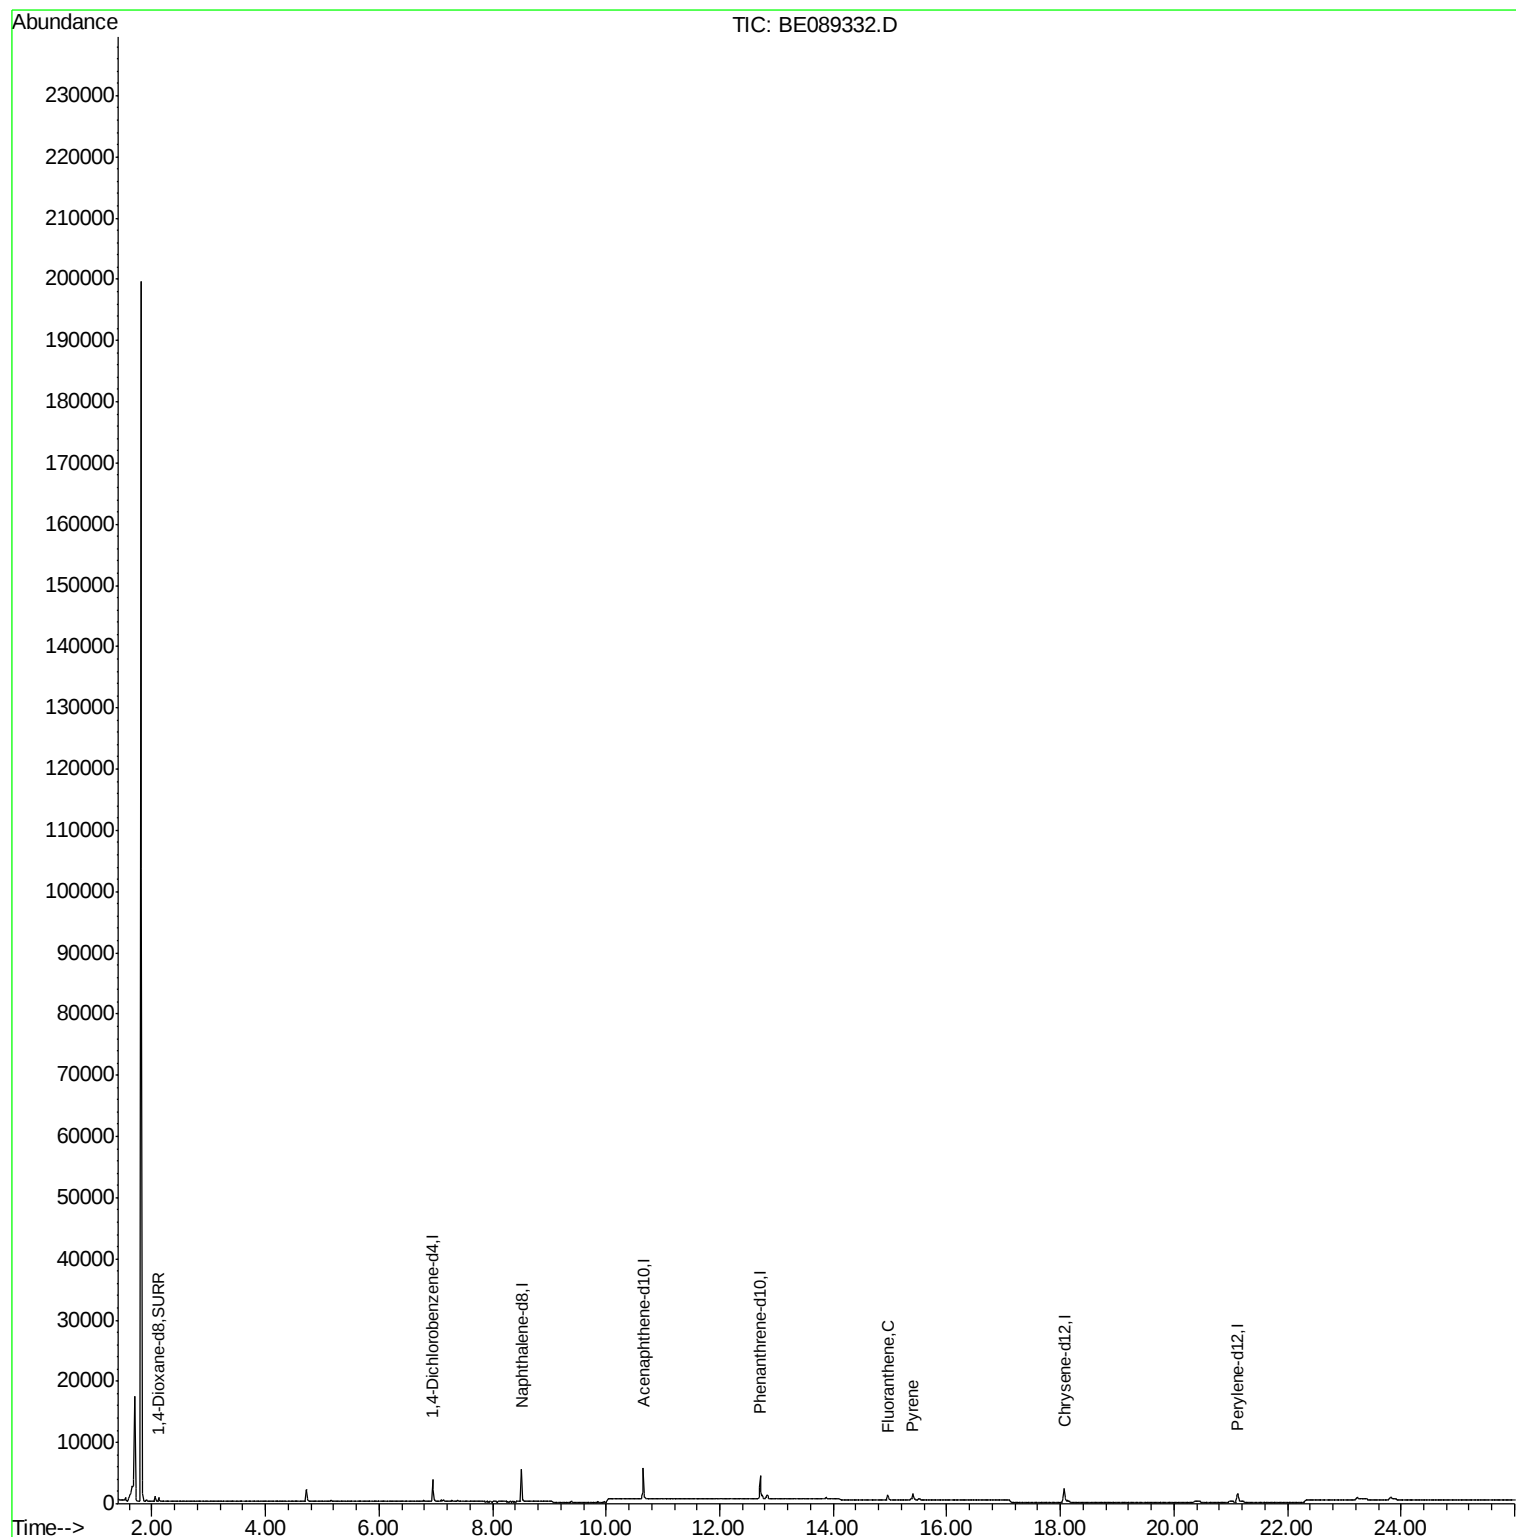


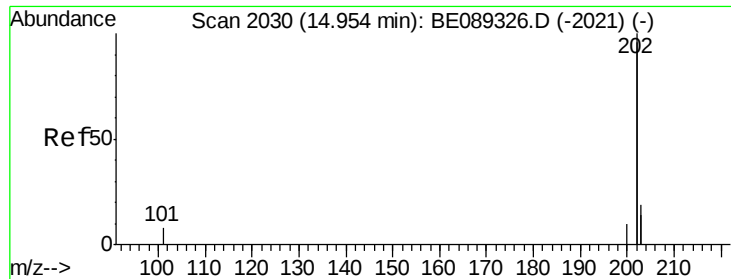

#17
Fluoranthene
Concen: 0.03 ng/ul
RT: 14.95 min Scan# 2029
Delta R.T. 0.01 min
Lab File: BE089332.D
Acq: 7 Jan 2015 14:37

Instrument :
BNA_E
ClientSampleId :
Y9RB5

Tgt Ion:202 Resp: 1299
Ion Ratio Lower Upper
202 100
101 10.0 0.0 24.6
203 33.3 0.0 37.8

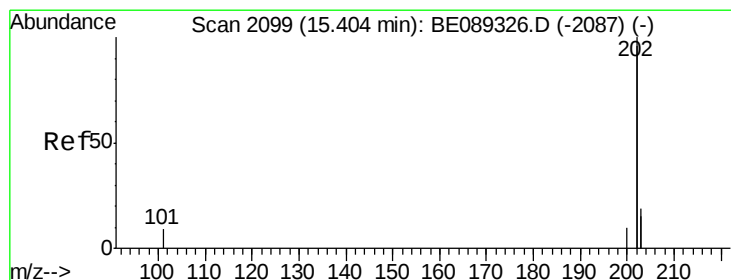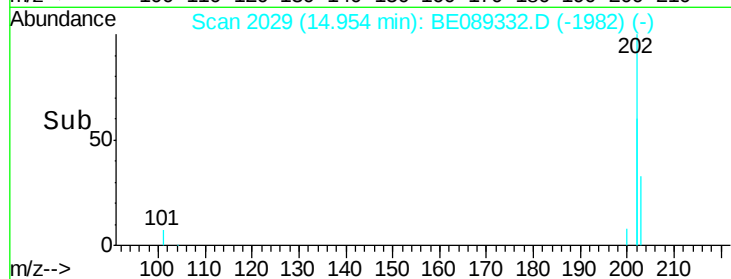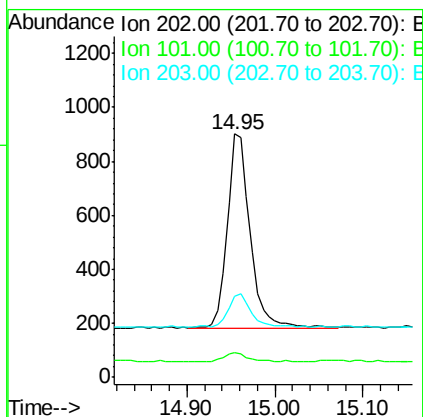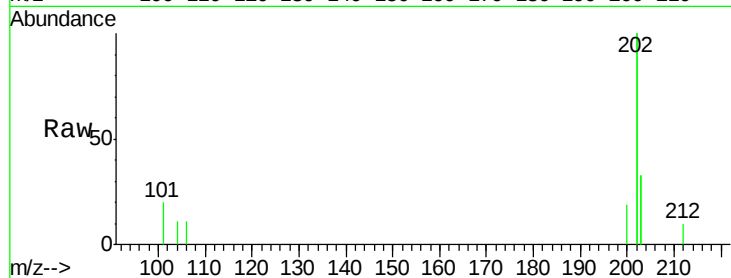

#19
Pyrene
Concen: 0.04 ng/ul
RT: 15.40 min Scan# 2098
Delta R.T. 0.01 min
Lab File: BE089332.D
Acq: 7 Jan 2015 14:37

Tgt Ion:202 Resp: 1371
Ion Ratio Lower Upper
202 100
200 8.8 4.2 6.4#
203 34.4 14.4 21.6#

