

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010715\
 Data File : BE089333.D
 Acq On : 7 Jan 2015 15:10
 Operator : TP/IZ
 Sample : F5245-20
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Y9RC5

Quant Time: Jan 08 13:08:07 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 08 01:37:38 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1158	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	4559	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.66	164	2381	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	3686	0.40	ng/ul	0.00
18) Chrysene-d12	18.07	240	2750	0.40	ng/ul	0.00
22) Perylene-d12	21.12	264	2358	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.11	96	522	0.30	ng/uL	0.00
6) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
17) Fluoranthene	14.96	202	1095	0.03	ng/ul	Qvalue 63
19) Pyrene	15.41	202	1080	0.03	ng/ul#	62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010715\
Data File : BE089333.D
Acq On : 7 Jan 2015 15:10
Operator : TP/IZ
Sample : F5245-20
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Y9RC5

Quant Time: Jan 08 13:08:07 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 08 01:37:38 2015
Response via : Initial Calibration




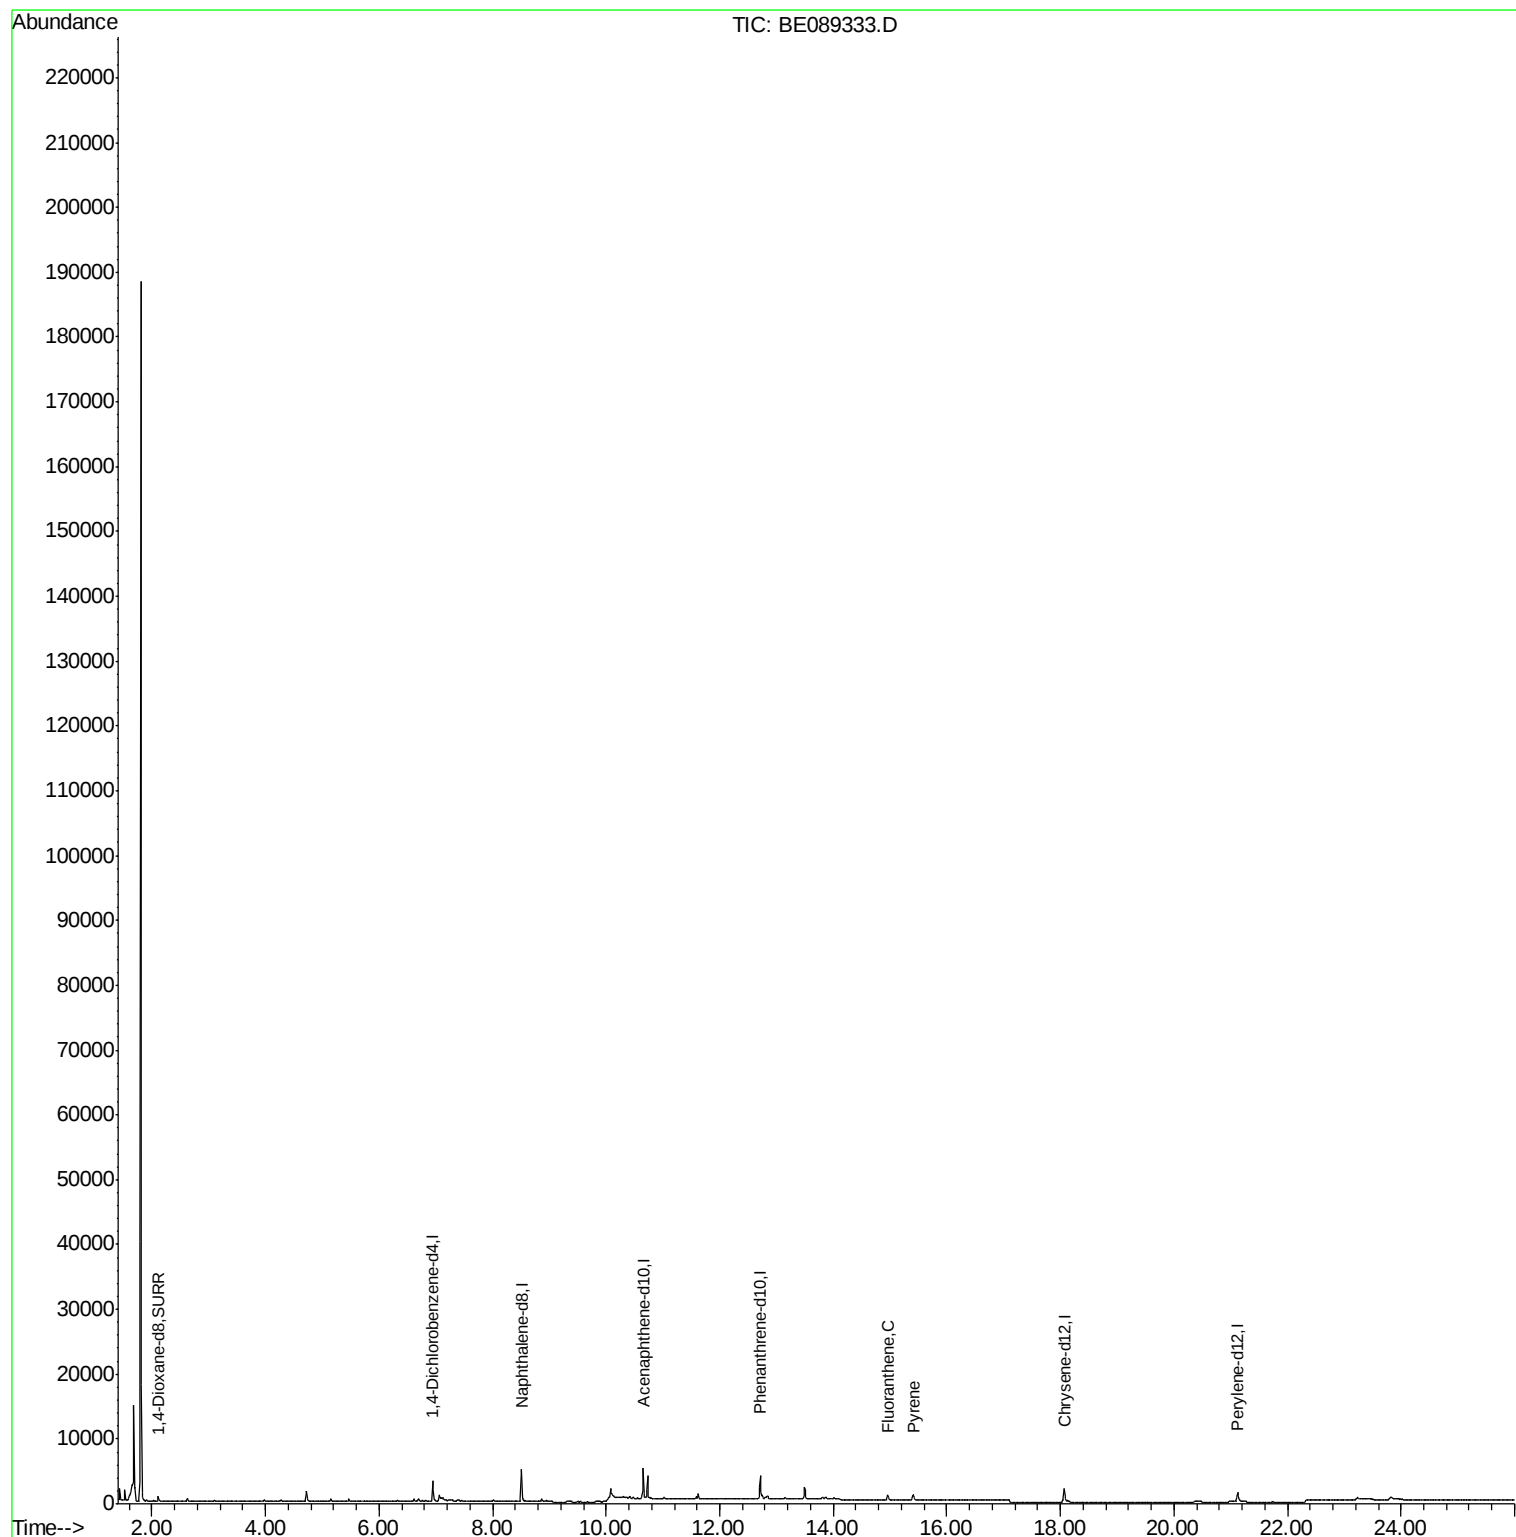


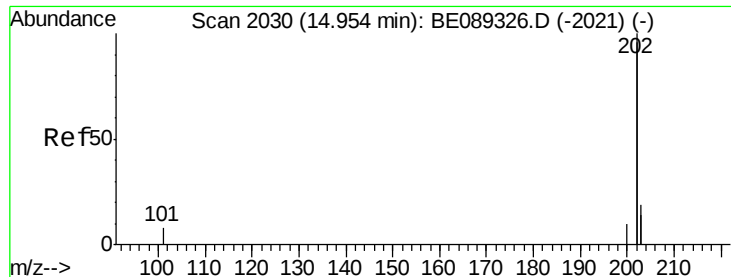

#17
Fluoranthene
 Concen: 0.03 ng/ul
 RT: 14.96 min Scan# 2031
 Delta R.T. 0.01 min
 Lab File: BE089333.D
 Acq: 7 Jan 2015 15:10

Instrument :
 BNA_E
 ClientSampleId :
 Y9RC5

Tgt Ion:202 Resp: 1095
 Ion Ratio Lower Upper
 202 100
 101 9.8 0.0 24.6
 203 36.4 0.0 37.8

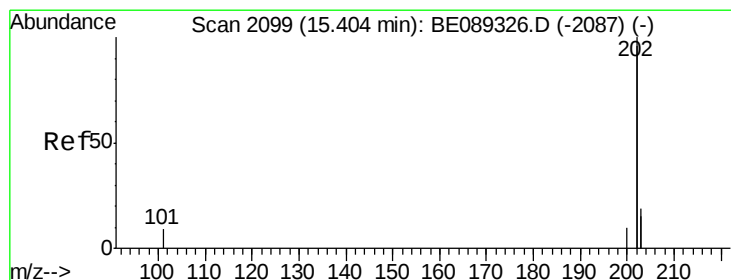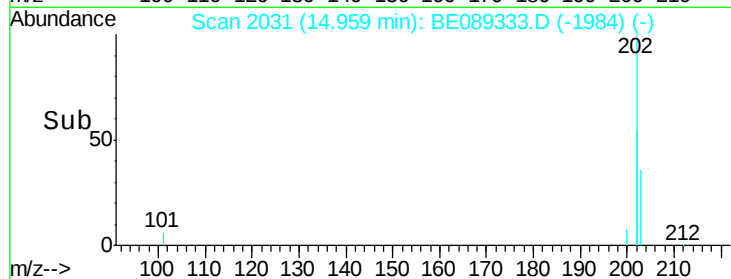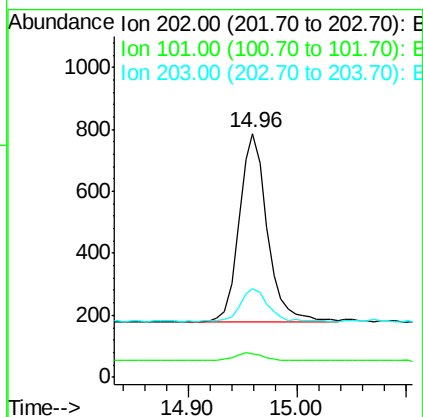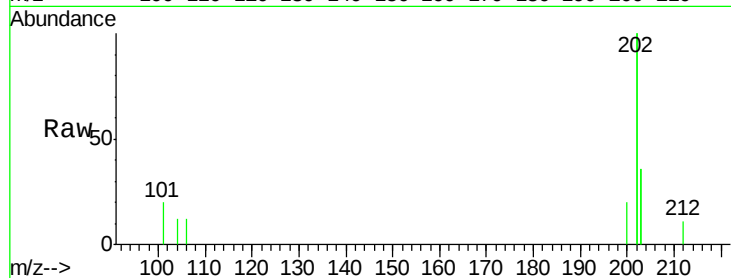

#19
Pyrene
 Concen: 0.03 ng/ul
 RT: 15.41 min Scan# 2100
 Delta R.T. 0.01 min
 Lab File: BE089333.D
 Acq: 7 Jan 2015 15:10

Tgt Ion:202 Resp: 1080
 Ion Ratio Lower Upper
 202 100
 200 9.8 4.2 6.4#
 203 38.0 14.4 21.6#

