


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010715\
 Data File : BE089335.D
 Acq On : 7 Jan 2015 18:12
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BASE-BE010715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 08 15:21:44 2015

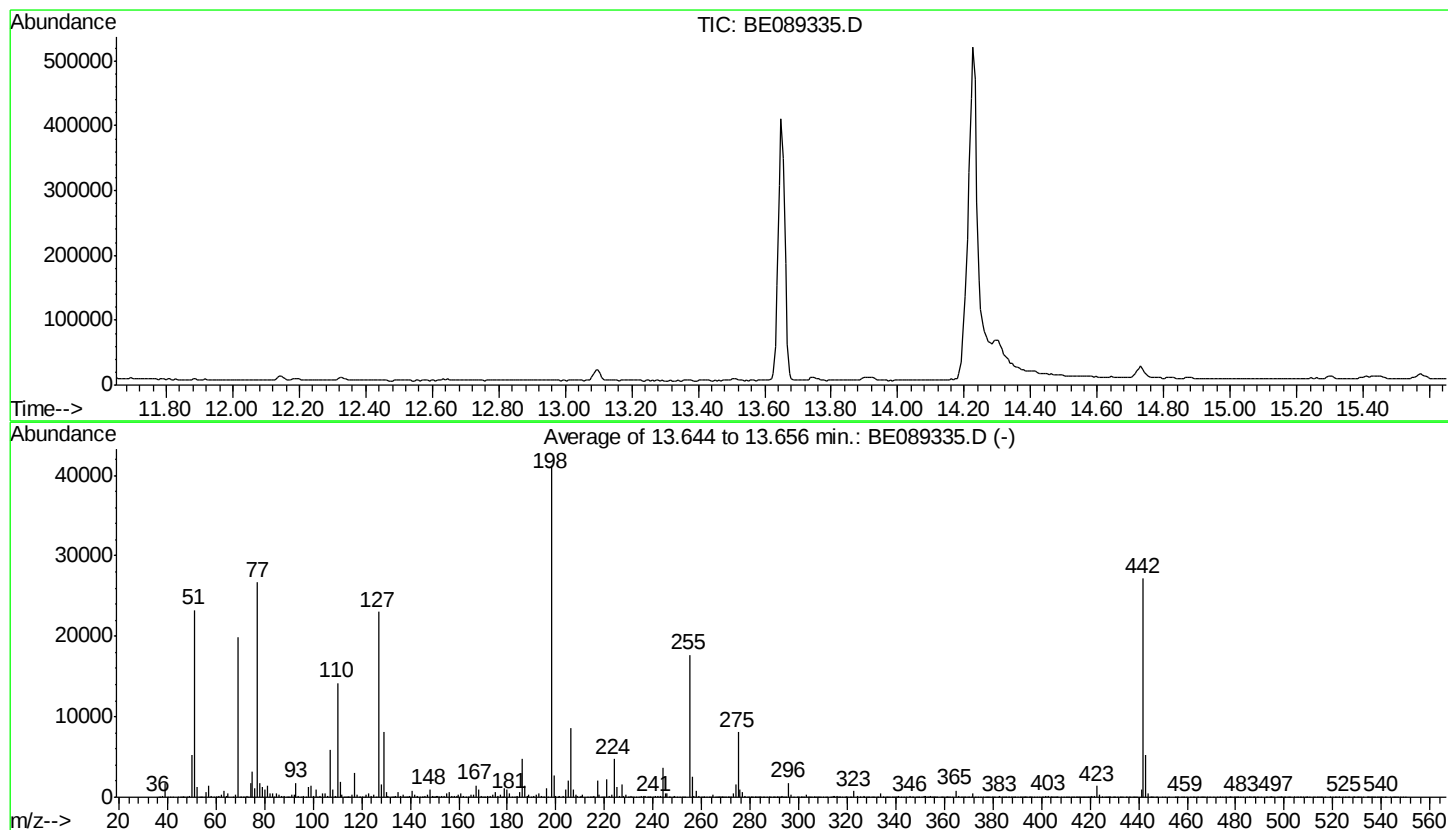

AutoFind: Scans 2086, 2087, 2088; Background Corrected with Scan 2077

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.4	23226	PASS
68	69	0.00	2	1.3	249	PASS
69	198	0.00	100	48.3	19895	PASS
70	69	0.00	2	0.2	48	PASS
127	198	10	80	55.9	23028	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41205	PASS
199	198	5	9	6.6	2732	PASS
275	198	10	60	19.5	8044	PASS
365	198	1	100	1.9	802	PASS
441	442	0.01	24	3.7	1010	PASS
442	198	50	100	65.8	27126	PASS
443	442	15	24	19.6	5326	PASS