

Data Path : Z:\HPCHEM1\BNA_E\Data\BE010815\
 Data File : BE089374.D
 Acq On : 8 Jan 2015 19:55
 Operator : TP/IZ
 Sample : F5245-19RX
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Y9RB5

Quant Time: Jan 09 03:07:50 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 09 01:27:36 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1016	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	3979	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.65	164	2137	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	3365	0.40	ng/ul	0.00
18) Chrysene-d12	18.07	240	2388	0.40	ng/ul	0.00
22) Perylene-d12	21.12	264	2045	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	2.11	96	448	0.29	ng/uL	0.00
6) 2-Methylnaphthalene-d10	0.00	152	0	0.00	ng/ul	
16) Fluoranthene-d10	14.94	212	1	0.00	ng/ul	0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) 1,4-Dioxane	1.80	88	5650	3.32	ng/ul#	1
5) Naphthalene	8.53	128	146	0.02	ng/ul#	39
7) 2-Methylnaphthalene	9.39	142	37	0.01	ng/ul	92
9) Acenaphthylene	10.48	152	100	0.00	ng/ul#	1
10) Acenaphthene	10.69	153	120	0.01	ng/ul#	45
11) Fluorene	11.34	166	23	0.00	ng/ul#	62
13) Pentachlorophenol	12.03	266	456	1.31	ng/ul#	25
14) Phenanthrene	12.75	178	582	0.02	ng/ul#	38
15) Anthracene	12.83	178	534	0.02	ng/ul#	35
17) Fluoranthene	14.95	202	1061	0.03	ng/ul	62
19) Pyrene	15.40	202	1117	0.04	ng/ul#	63
20) Benzo(a)anthracene	18.05	228	254	0.05	ng/ul#	62
21) Chrysene	18.12	228	268	0.04	ng/ul#	61
23) Benzo(b)fluoranthene	20.37	252	175	0.03	ng/ul#	25
24) Benzo(k)fluoranthene	20.43	252	244	0.04	ng/ul#	29
25) Benzo(a)pyrene	21.01	252	192	0.04	ng/ul#	23
26) Indeno(1,2,3-cd)pyrene	23.23	276	477	0.03	ng/ul#	94
27) Dibenzo(a,h)anthracene	23.31	278	142	0.03	ng/ul#	21
28) Benzo(g,h,i)perylene	23.82	276	737	0.04	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\Data\BE010815\
Data File : BE089374.D
Acq On : 8 Jan 2015 19:55
Operator : TP/IZ
Sample : F5245-19RX
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Y9RB5

Quant Time: Jan 09 03:07:50 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 09 01:27:36 2015
Response via : Initial Calibration

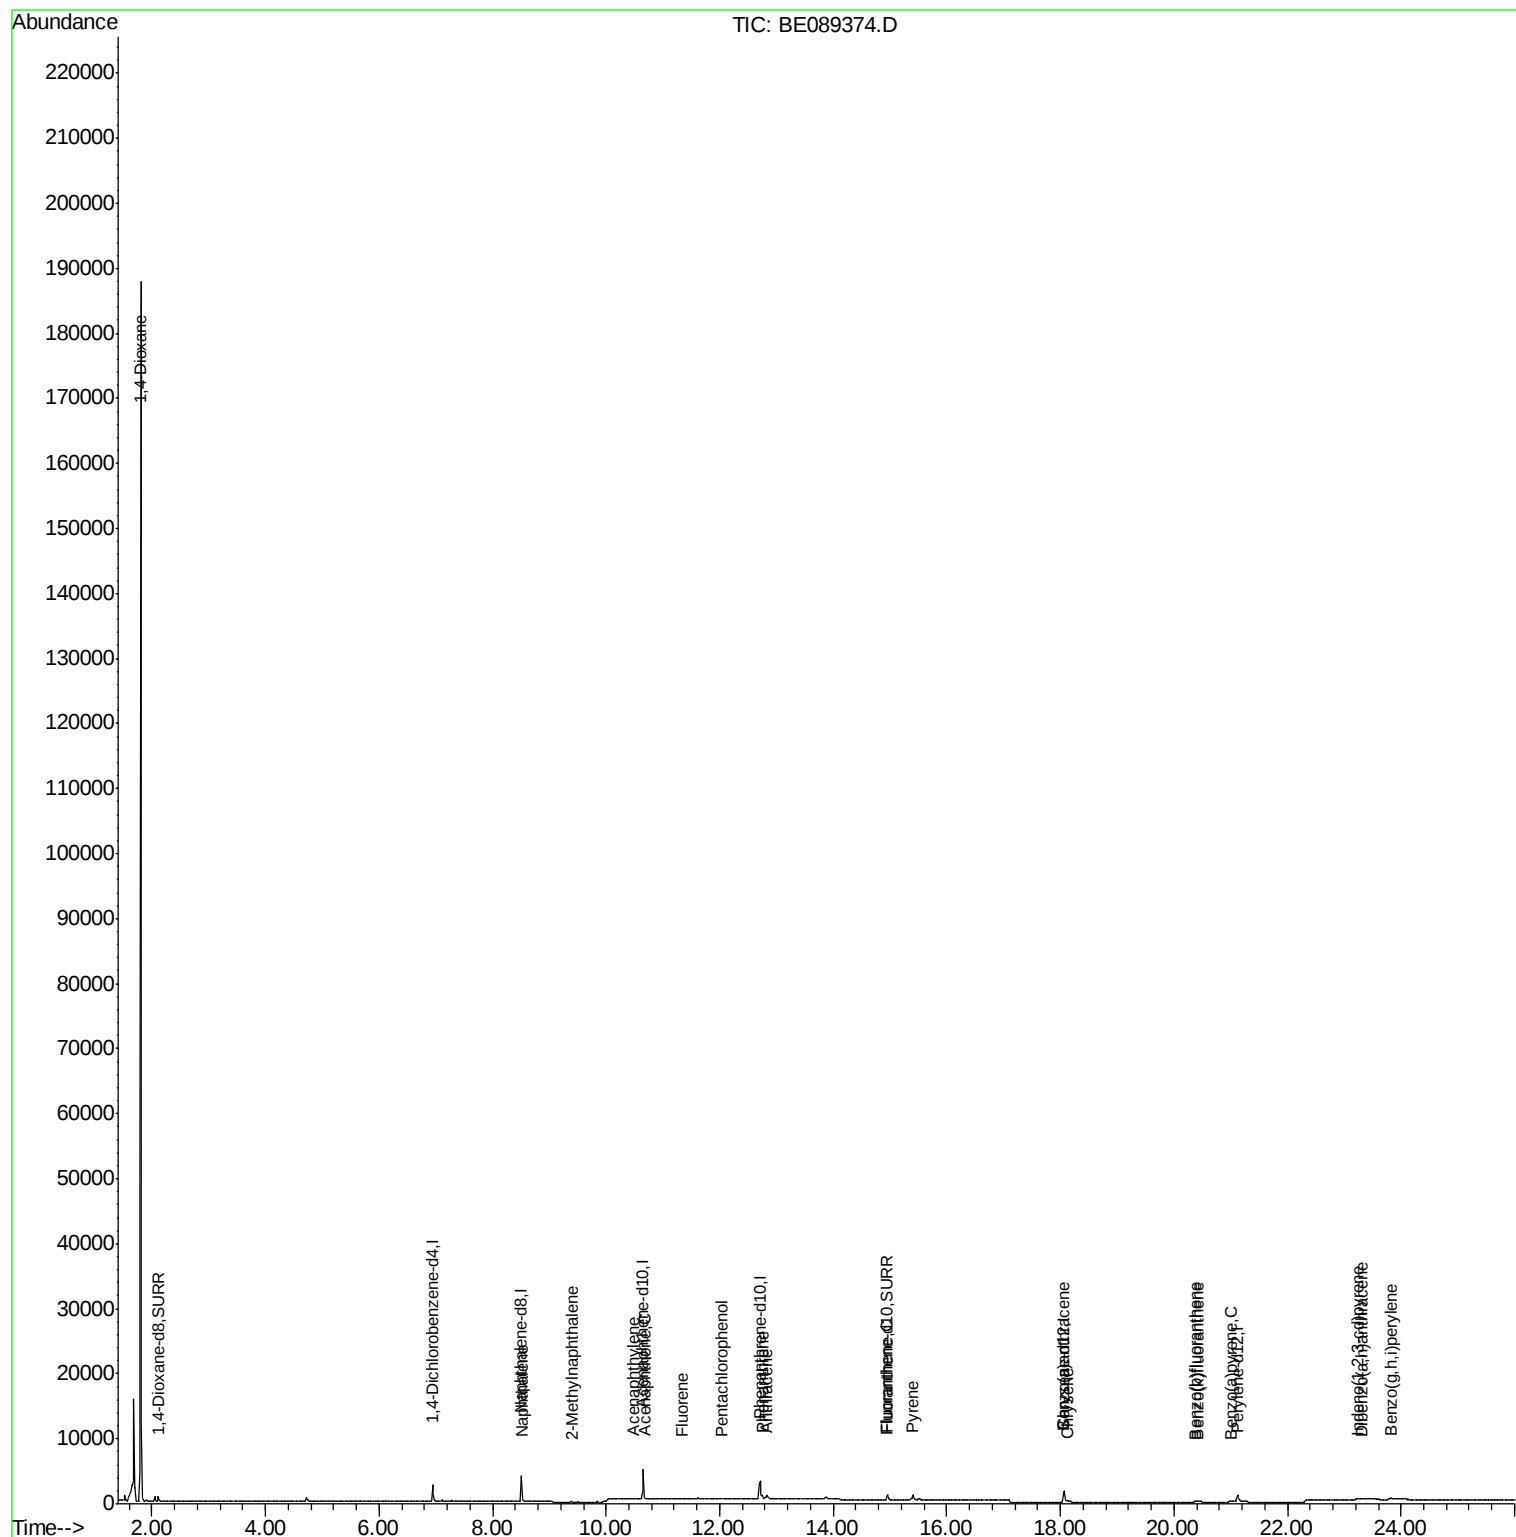

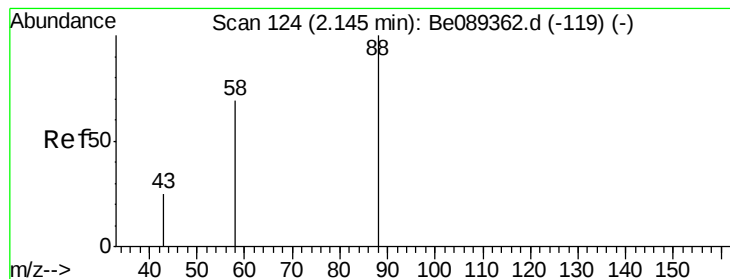

#3

1,4-Dioxane

Concen: 3.32 ng/ul

RT: 1.80 min Scan# 67

Delta R.T. -0.34 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :

Y9RB5





Tgt Ion: 88 Resp: 5650

Ion Ratio Lower Upper

88 100

58 29.3 61.5 92.3#

43 3049.2 23.9 35.9#

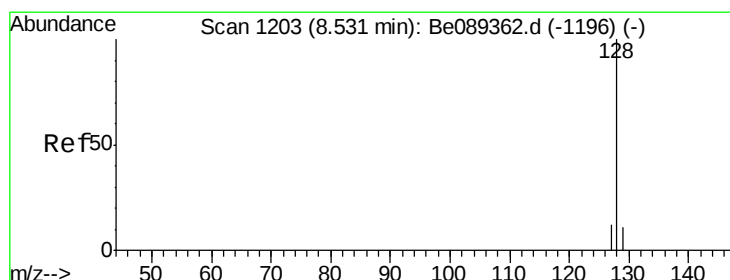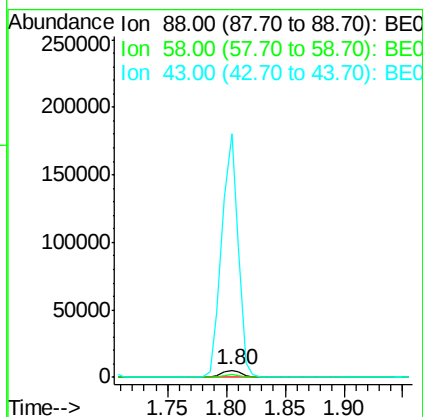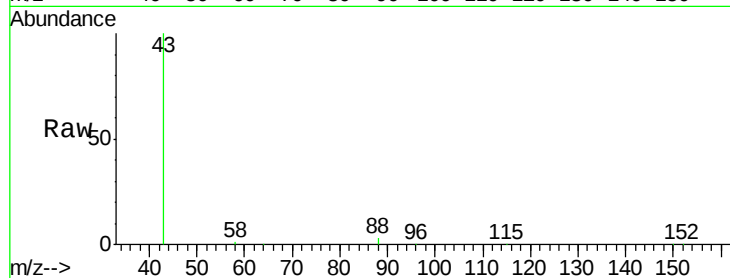

#5

Naphthalene

Concen: 0.02 ng/ul

RT: 8.53 min Scan# 1203

Delta R.T. 0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55




Tgt Ion: 128 Resp: 146


Ion Ratio Lower Upper

128 100

129 34.9 9.1 13.7#

127 36.1 10.0 15.0#

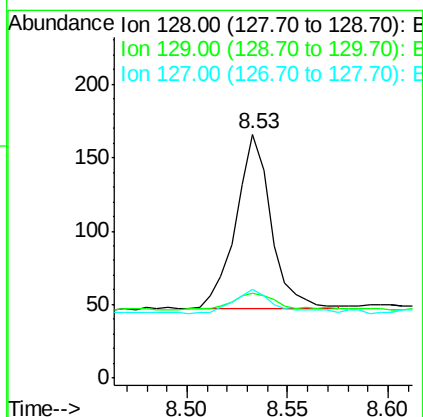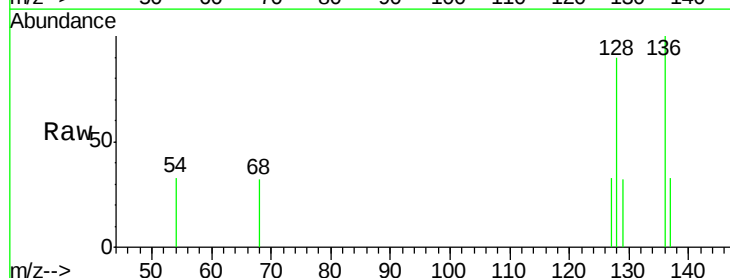

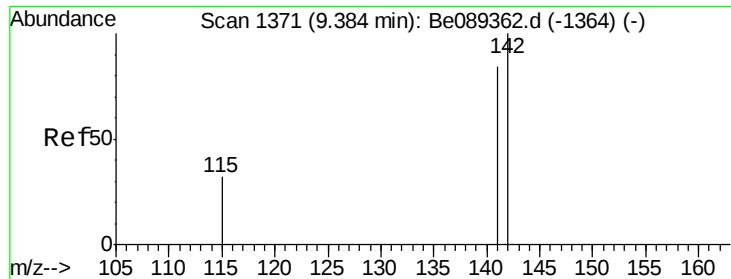

#7

2-Methylnaphthalene

Concen: 0.01 ng/ul

RT: 9.39 min Scan# 1371

Delta R.T. 0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :


Y9RB5

Tgt Ion:142 Resp: 37

Ion Ratio Lower Upper

142 100

141 89.2 65.4 98.0

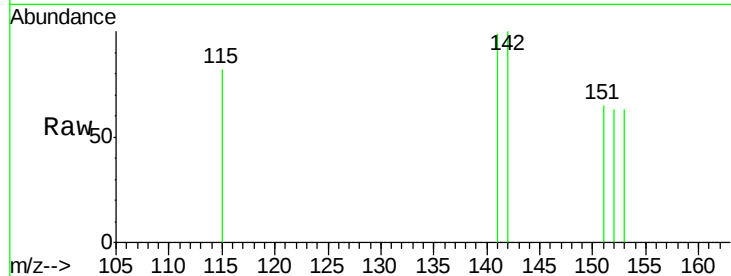

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

9.39

80



60

40

20

0

Time--> 9.35 9.40 9.45

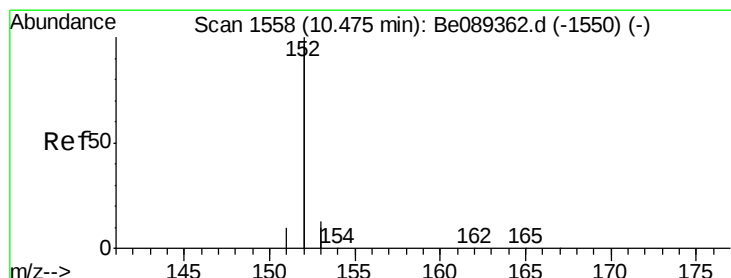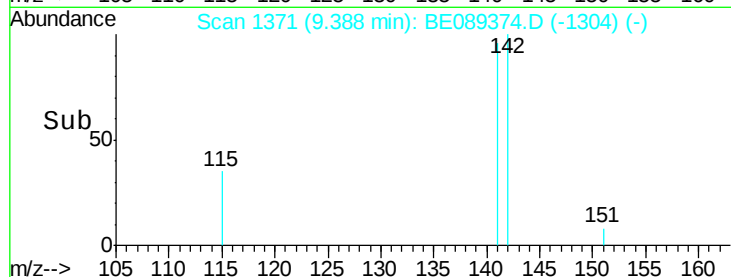

#9

Acenaphthylene

Concen: 0.00 ng/ul

RT: 10.48 min Scan# 1558

Delta R.T. 0.01 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55


Tgt Ion:152 Resp: 100

Ion Ratio Lower Upper

152 100

151 22.7 4.0 6.0#

153 83.5 10.1 15.1#

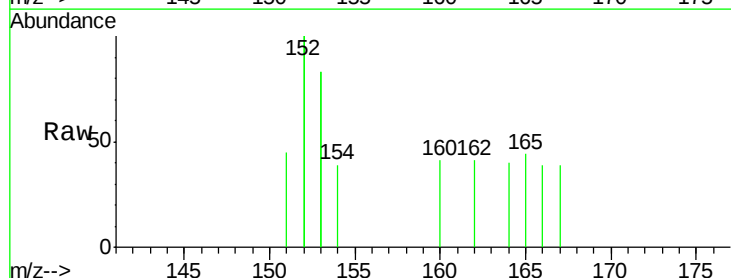

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

10.48

300

250

200


150


100

50

0

Time--> 10.40 10.45 10.50 10.55

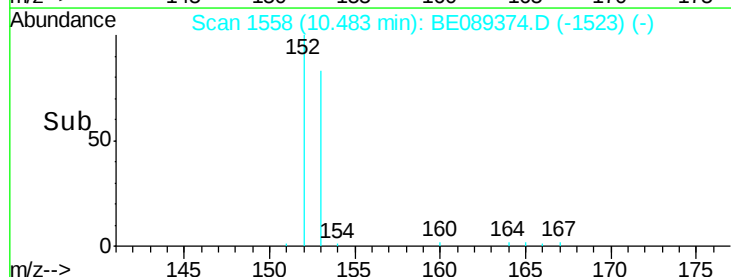

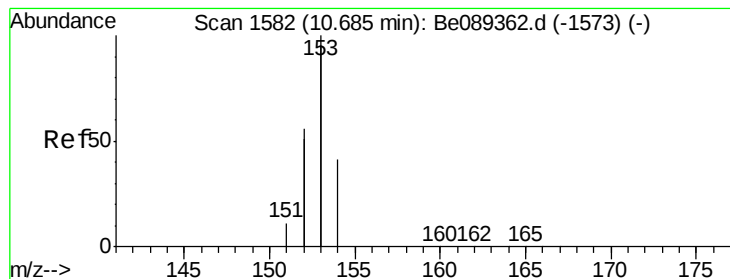

#10

Acenaphthene

Concen: 0.01 ng/ul

RT: 10.69 min Scan# 1582

Delta R.T. 0.01 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :

Y9RB5


Tgt Ion:153 Resp: 120

Ion Ratio Lower Upper


153 100

152 94.7 32.6 49.0#



154 23.7 21.8 32.6

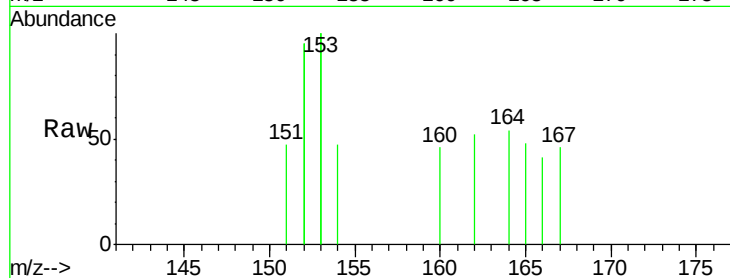

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

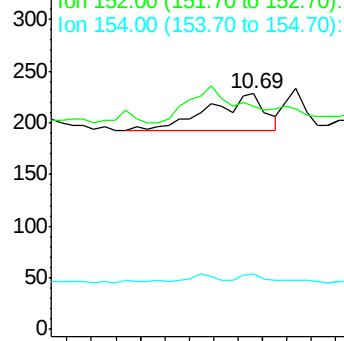

Time-->

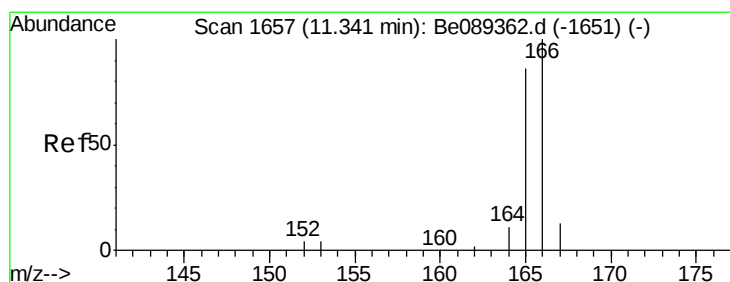

#11

Fluorene

Concen: 0.00 ng/ul

RT: 11.34 min Scan# 1656

Delta R.T. -0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55


Tgt Ion:166 Resp: 23

Ion Ratio Lower Upper


166 100

165 104.9 70.3 105.5


167 80.3 11.5 17.3#

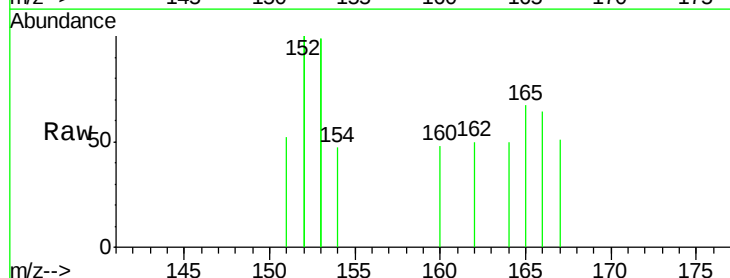


Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

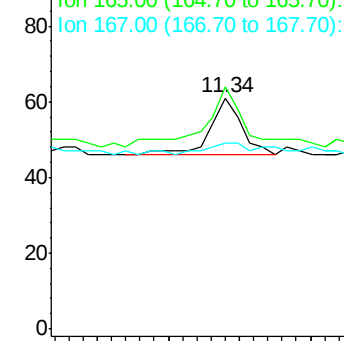

Time-->





#13

Pentachlorophenol

Concen: 1.31 ng/ul

RT: 12.03 min Scan# 1732

Delta R.T. -0.24 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :

Y9RB5


Tgt Ion: 266 Resp: 456

Ion Ratio Lower Upper

266 100

264 148.0 48.7 73.1#




268 96.5 52.9 79.3#

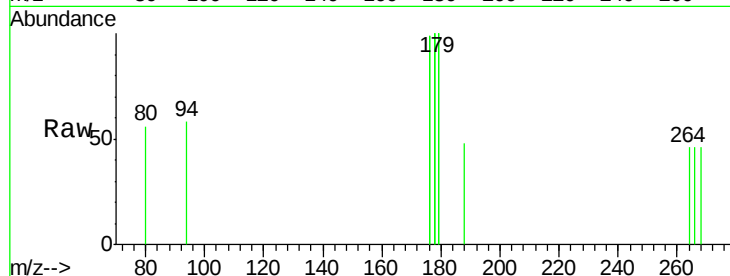

Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

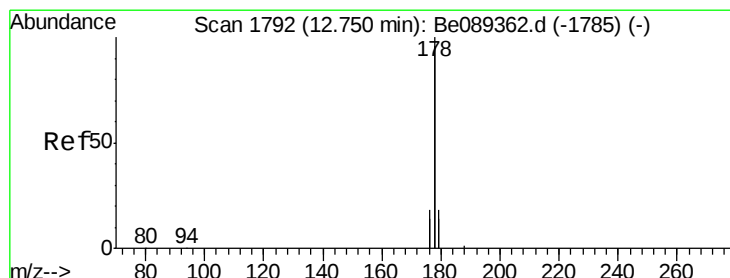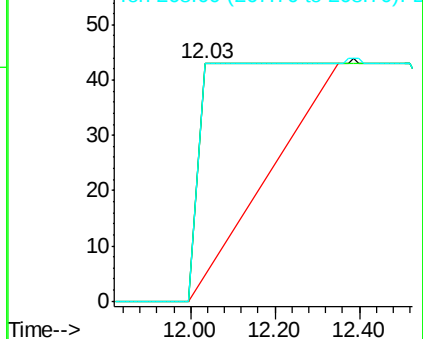

#14

Phenanthrene

Concen: 0.02 ng/ul

RT: 12.75 min Scan# 1791

Delta R.T. -0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55


Tgt Ion: 178 Resp: 582

Ion Ratio Lower Upper

178 100

176 45.0 14.3 21.5#



179 44.6 13.8 20.8#

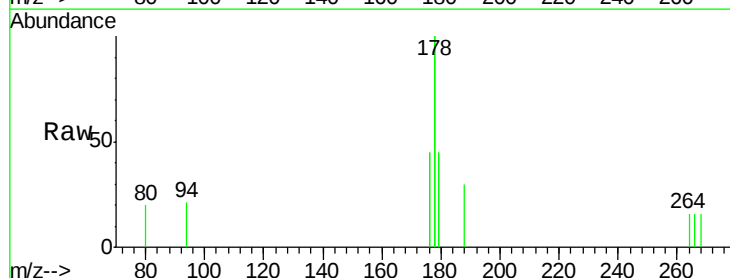


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

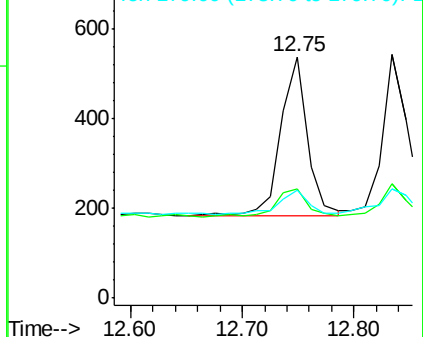

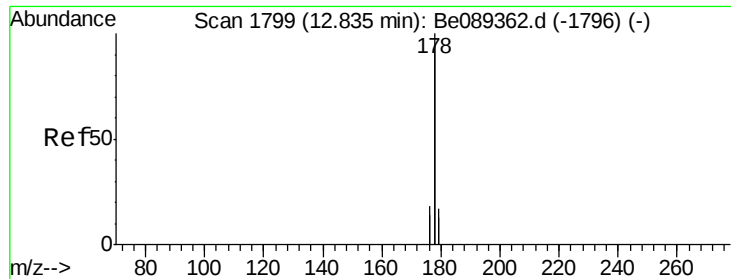

#15

Anthracene

Concen: 0.02 ng/ul

RT: 12.83 min Scan# 1798

Delta R.T. -0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :

Y9RB5





Tgt Ion:178 Resp: 534

Ion Ratio Lower Upper

178 100

176 46.9 14.7 22.1#

179 45.0 13.4 20.2#

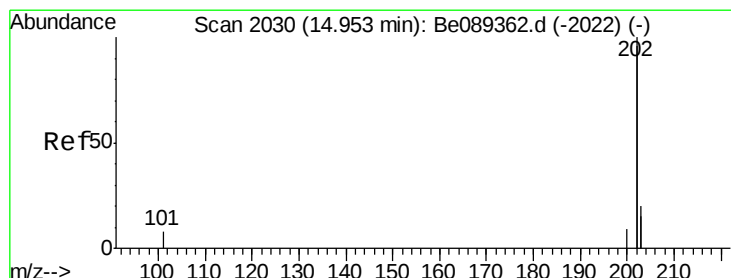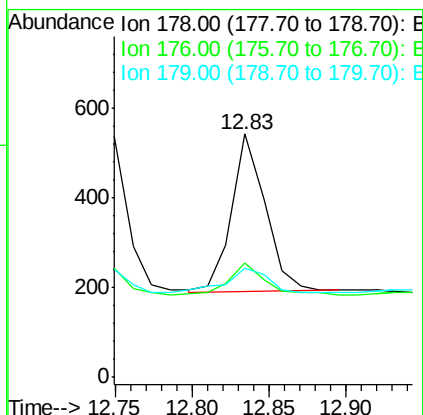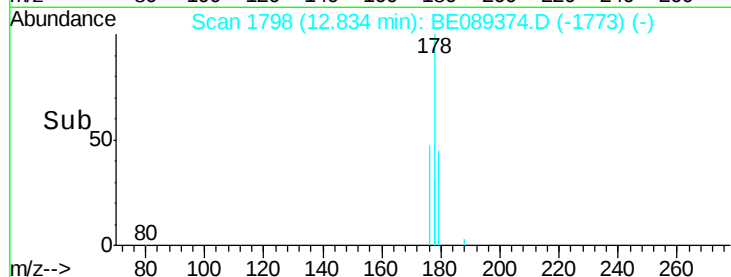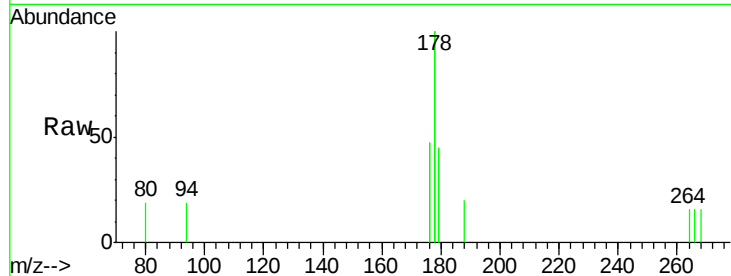

#17

Fluoranthene

Concen: 0.03 ng/ul

RT: 14.95 min Scan# 2029

Delta R.T. 0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55




Tgt Ion:202 Resp: 1061


Ion Ratio Lower Upper

202 100

101 10.3 0.0 24.6

203 36.9 0.0 37.8

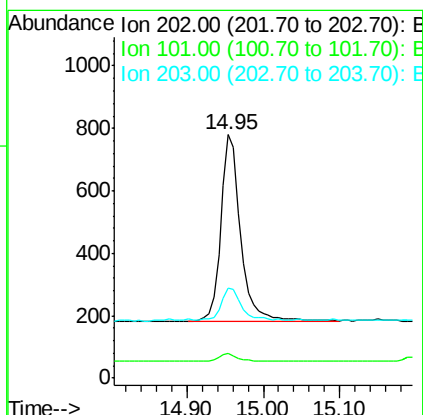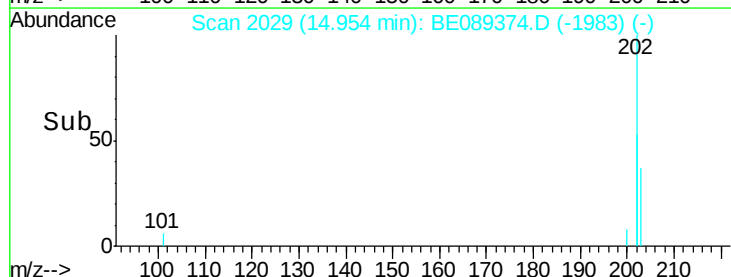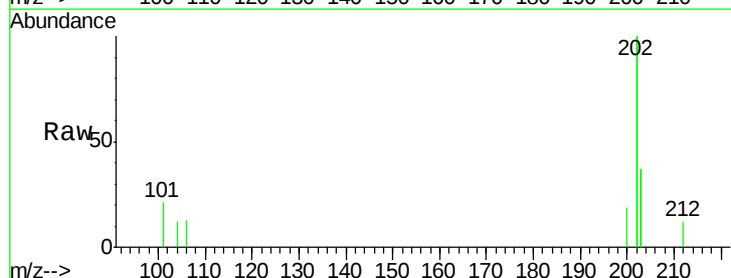

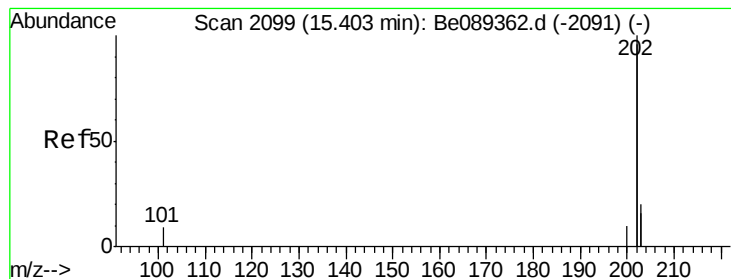

#19

Pyrene

Concen: 0.04 ng/ul

RT: 15.40 min Scan# 2098

Delta R.T. 0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampled :

Y9RB5


Tgt Ion:202 Resp: 1117

Ion Ratio Lower Upper

202 100

200 10.0 4.2 6.4#




203 37.3 14.4 21.6#

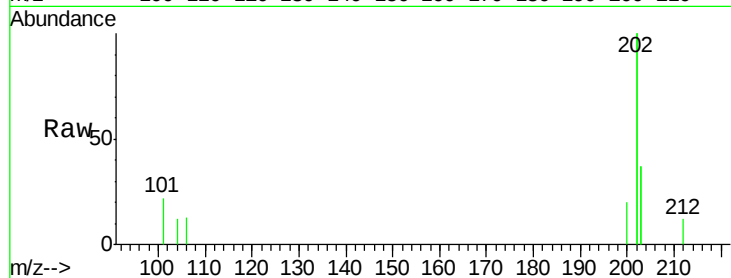

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

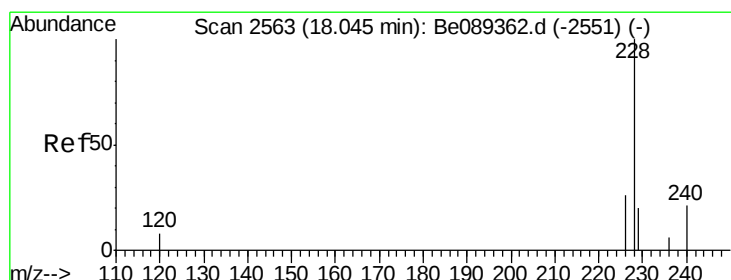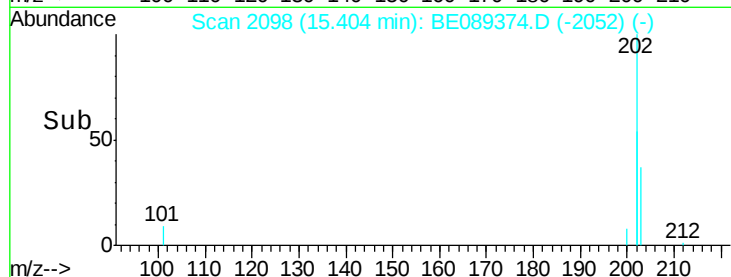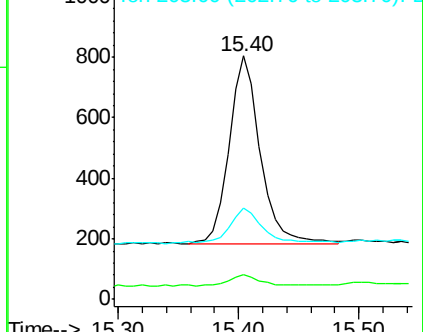

#20

Benzo(a)anthracene

Concen: 0.05 ng/ul

RT: 18.05 min Scan# 2563

Delta R.T. 0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55


Tgt Ion:228 Resp: 254

Ion Ratio Lower Upper

228 100

226 44.8 21.9 32.9#



229 41.4 16.9 25.3#

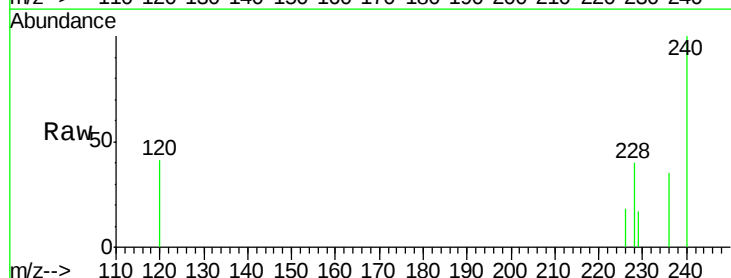


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

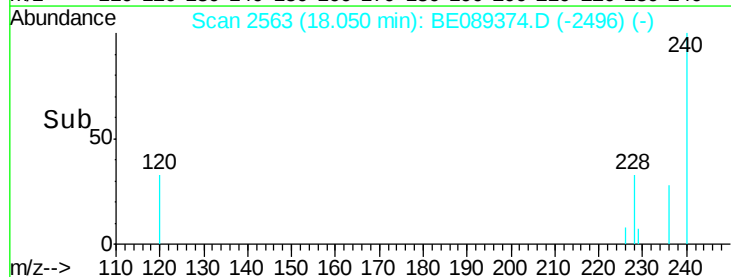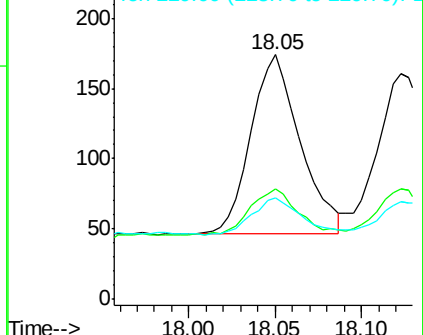

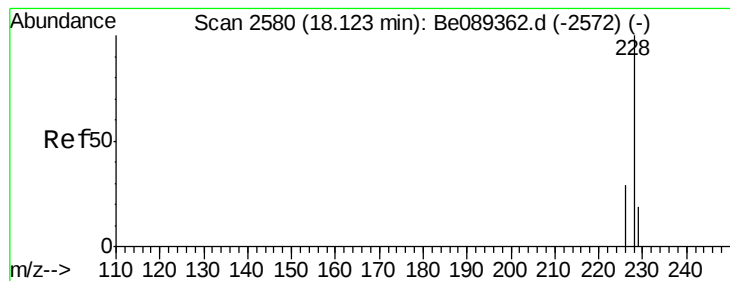

#21

Chrysene

Concen: 0.04 ng/ul

RT: 18.12 min Scan# 2579

Delta R.T. 0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :

Y9RB5


Tgt Ion:228 Resp: 268

Ion Ratio Lower Upper

228 100

226 48.4 23.9 35.9#




229 42.9 16.8 25.2#

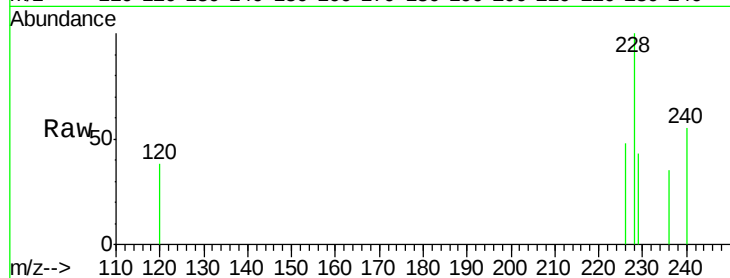

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

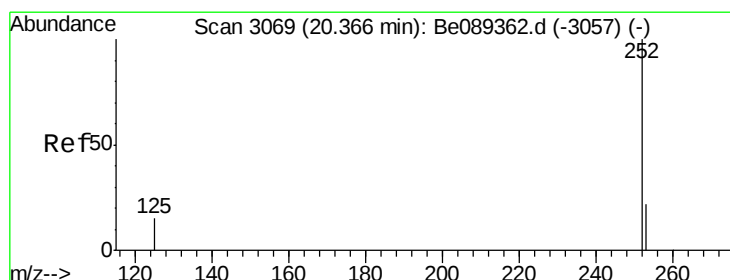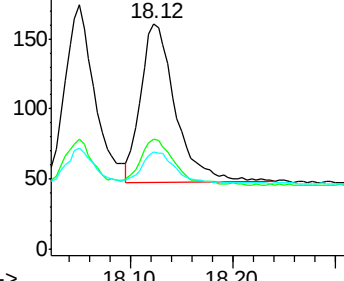

#23

Benzo(b)fluoranthene

Concen: 0.03 ng/ul

RT: 20.37 min Scan# 3069

Delta R.T. 0.01 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55


Tgt Ion:252 Resp: 175

Ion Ratio Lower Upper

252 100

253 51.2 0.0 47.8#



125 62.0 0.0 34.2#

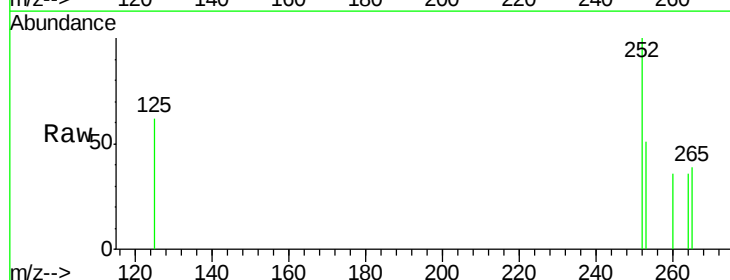


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

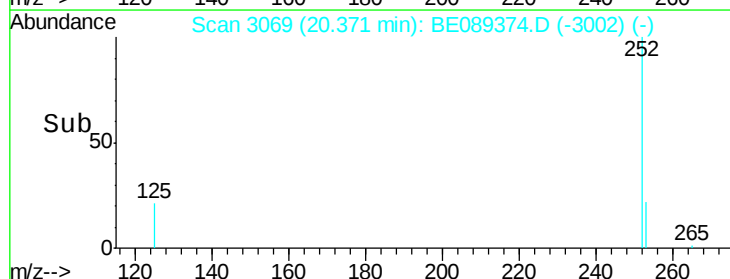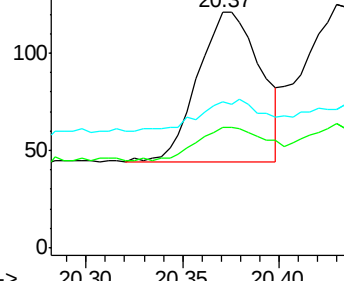

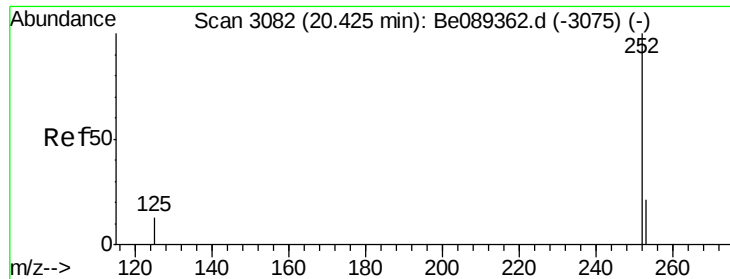

#24

Benzo(k)fluoranthene

Concen: 0.04 ng/ul

RT: 20.43 min Scan# 3082

Delta R.T. 0.01 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :

Y9RB5


Tgt Ion:252 Resp: 244

Ion Ratio Lower Upper

252 100

253 51.2 19.0 28.6#




125 56.8 13.5 20.3#

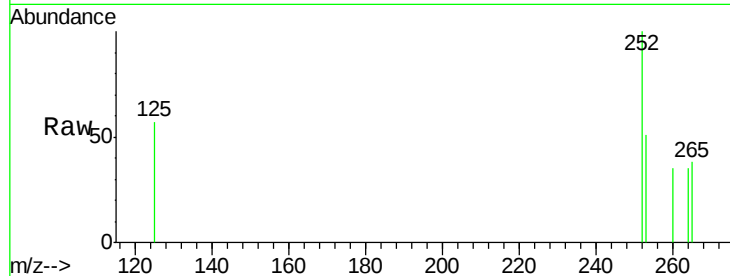

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

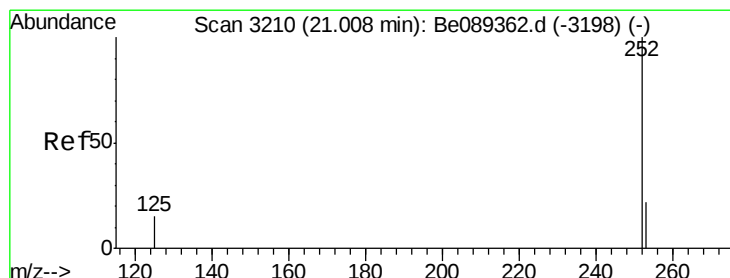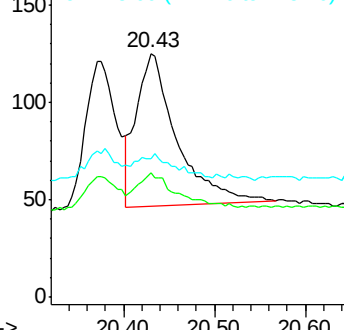

#25

Benzo(a)pyrene

Concen: 0.04 ng/ul

RT: 21.01 min Scan# 3209

Delta R.T. 0.00 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55


Tgt Ion:252 Resp: 192

Ion Ratio Lower Upper

252 100

253 53.6 19.7 29.5#



125 64.3 15.0 22.6#

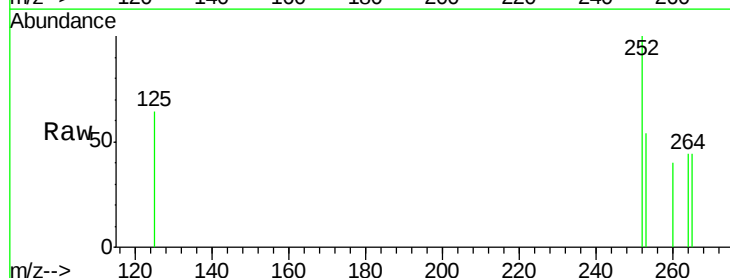


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

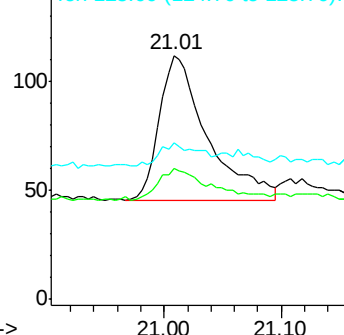

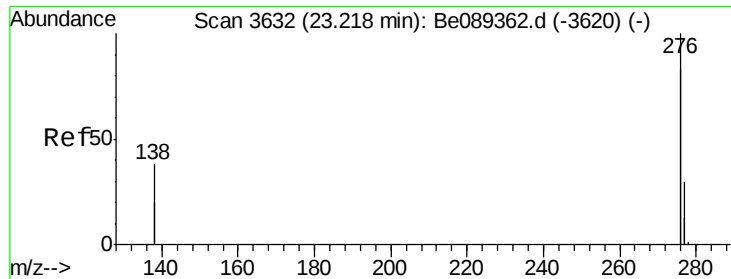

#26

Indeno(1,2,3-cd)pyrene

Concen: 0.03 ng/ul

RT: 23.23 min Scan# 3632

Delta R.T. 0.01 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :

Y9RB5


Tgt Ion: 276 Resp: 477

Ion Ratio Lower Upper

276 100

138 28.1 23.8 35.8




277 28.5 18.9 28.3#

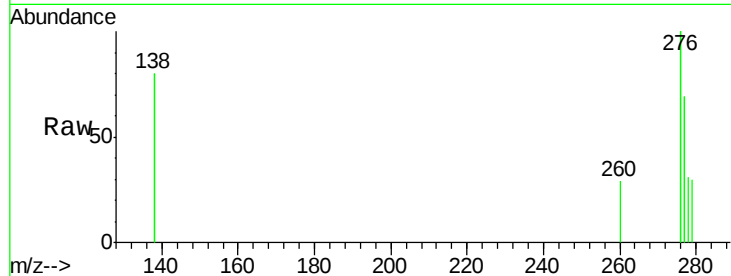

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

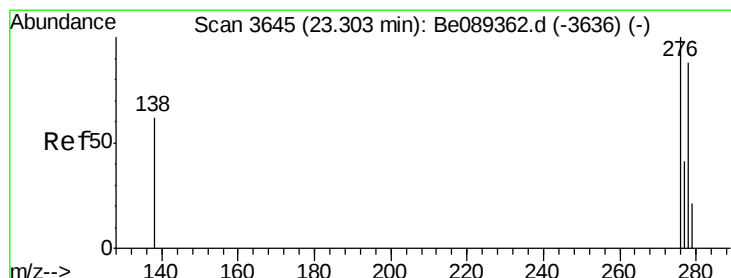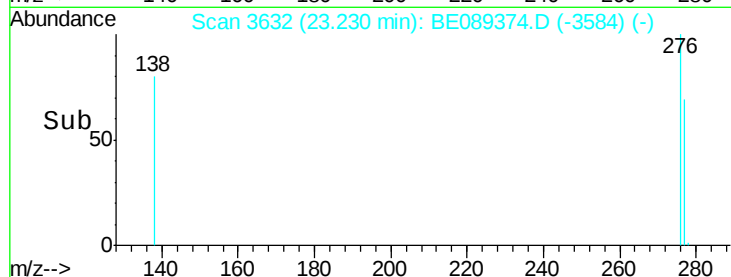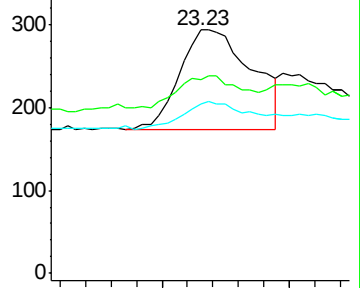

#27

Dibenzo(a,h)anthracene

Concen: 0.03 ng/ul

RT: 23.31 min Scan# 3645

Delta R.T. 0.01 min

Lab File: BE089374.D

Acq: 8 Jan 2015 19:55


Tgt Ion: 278 Resp: 142

Ion Ratio Lower Upper

278 100

139 0.0 0.0 0.0



279 72.9 24.0 36.0#

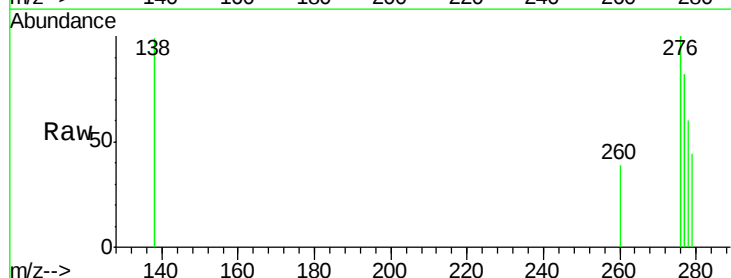


Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

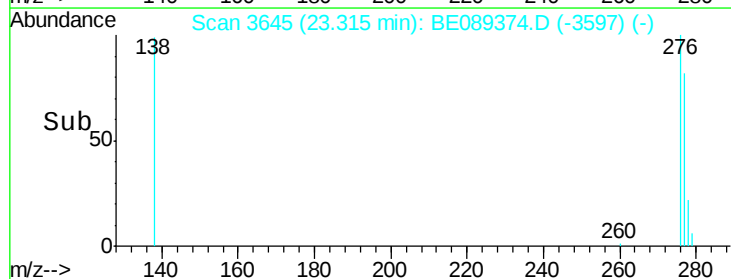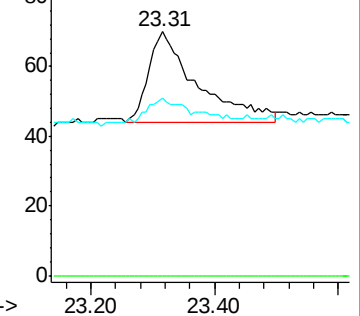

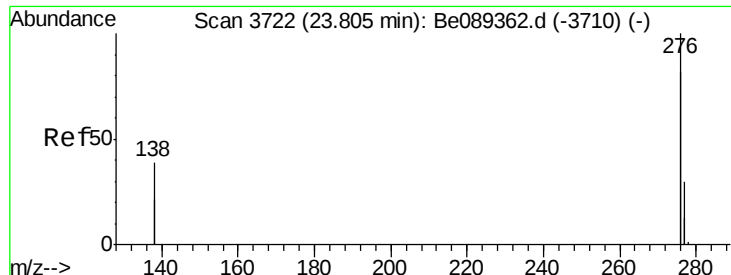

#28

Benzo(g,h,i)perylene

Concen: 0.04 ng/ul

RT: 23.82 min Scan# 3723

Delta R.T. 0.02 min

Lab File: BE089374.D


Acq: 8 Jan 2015 19:55

Instrument :

BNA_E

ClientSampleId :

Y9RB5

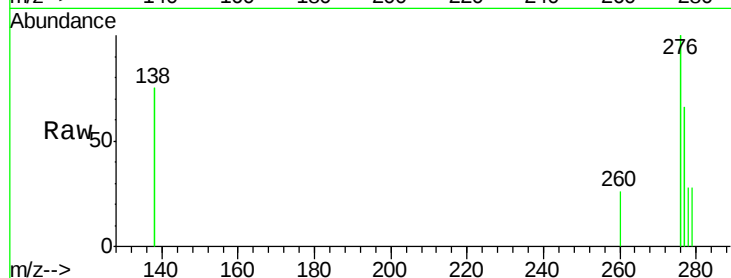


Tgt Ion: 276 Resp: 737

Ion Ratio Lower Upper

276 100

277 65.6 22.3 33.5#

138 75.5 30.0 45.0#

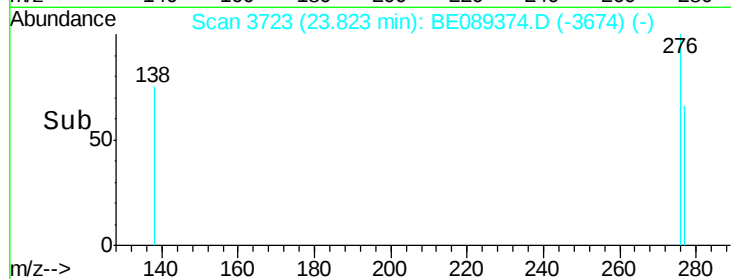

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

