


Data Path : Z:\HPCHEM1\BNA\_E\Data\BE010815\  
Data File : BE089377.D  
Acq On : 8 Jan 2015 23:27  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA\_E\METHODS\SOM01.2-EPA-SIM-BE123014.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Jan 09 01:27:36 2015

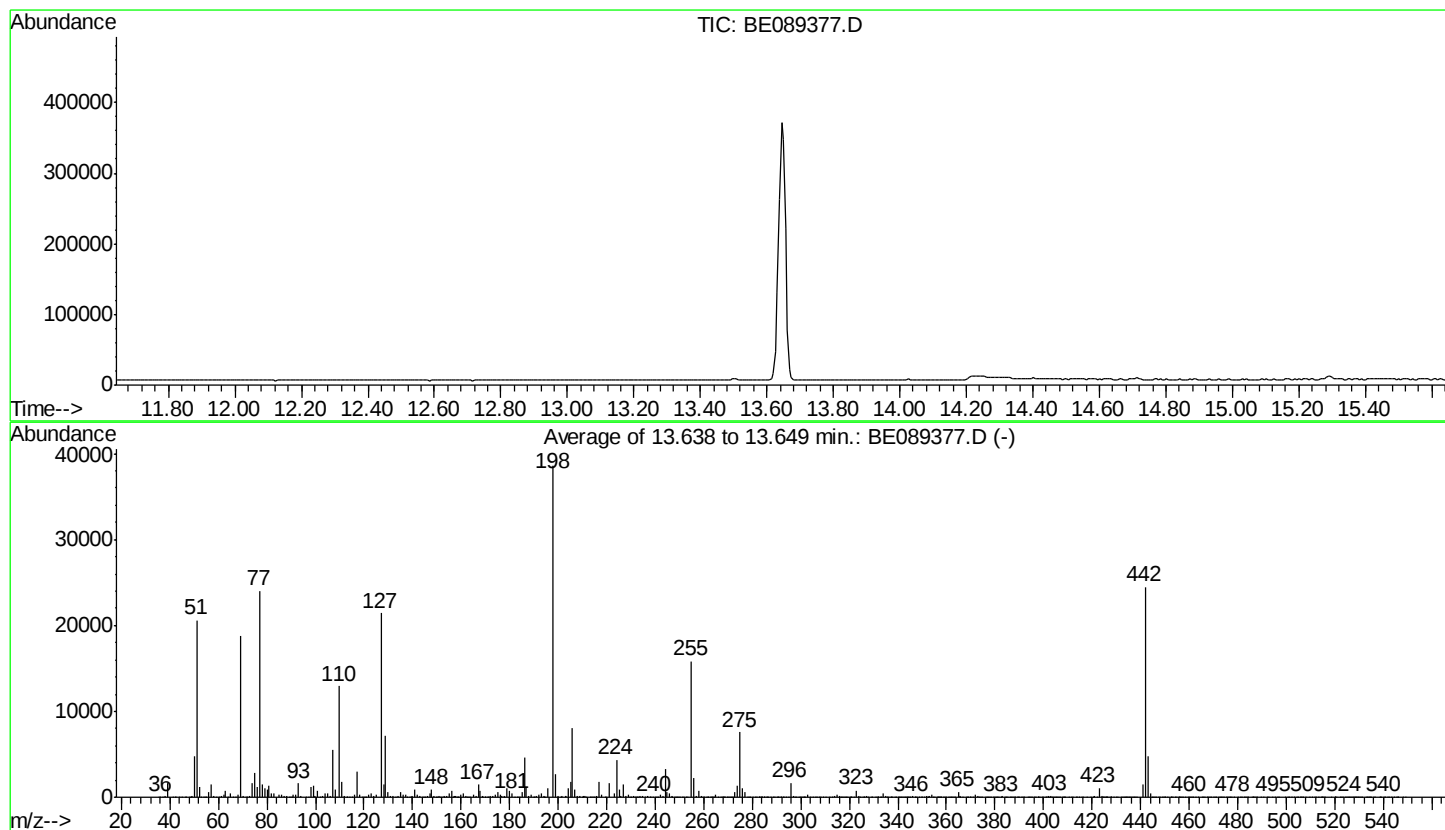

AutoFind: Scans 2085, 2086, 2087; Background Corrected with Scan 2076

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 53.3      | 20572   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.5       | 285     | PASS             |
| 69          | 198          | 0.00         | 100          | 48.8      | 18842   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 120     | PASS             |
| 127         | 198          | 10           | 80           | 55.4      | 21398   | PASS             |
| 197         | 198          | 0.00         | 1            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 38607   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 2652    | PASS             |
| 275         | 198          | 10           | 60           | 19.5      | 7532    | PASS             |
| 365         | 198          | 1            | 100          | 1.7       | 663     | PASS             |
| 441         | 443          | 0.01         | 100          | 32.3      | 1547    | PASS             |
| 442         | 198          | 50           | 100          | 63.4      | 24487   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 4792    | PASS             |