


Data Path : Z:\HPCHEM1\BNA_E\Data\BE010815\
 Data File : Be089361.d
 Acq On : 8 Jan 2015 12:24
 Operator : TP/IZ
 Sample : DFTPP37
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP37

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 02 10:52:56 2015

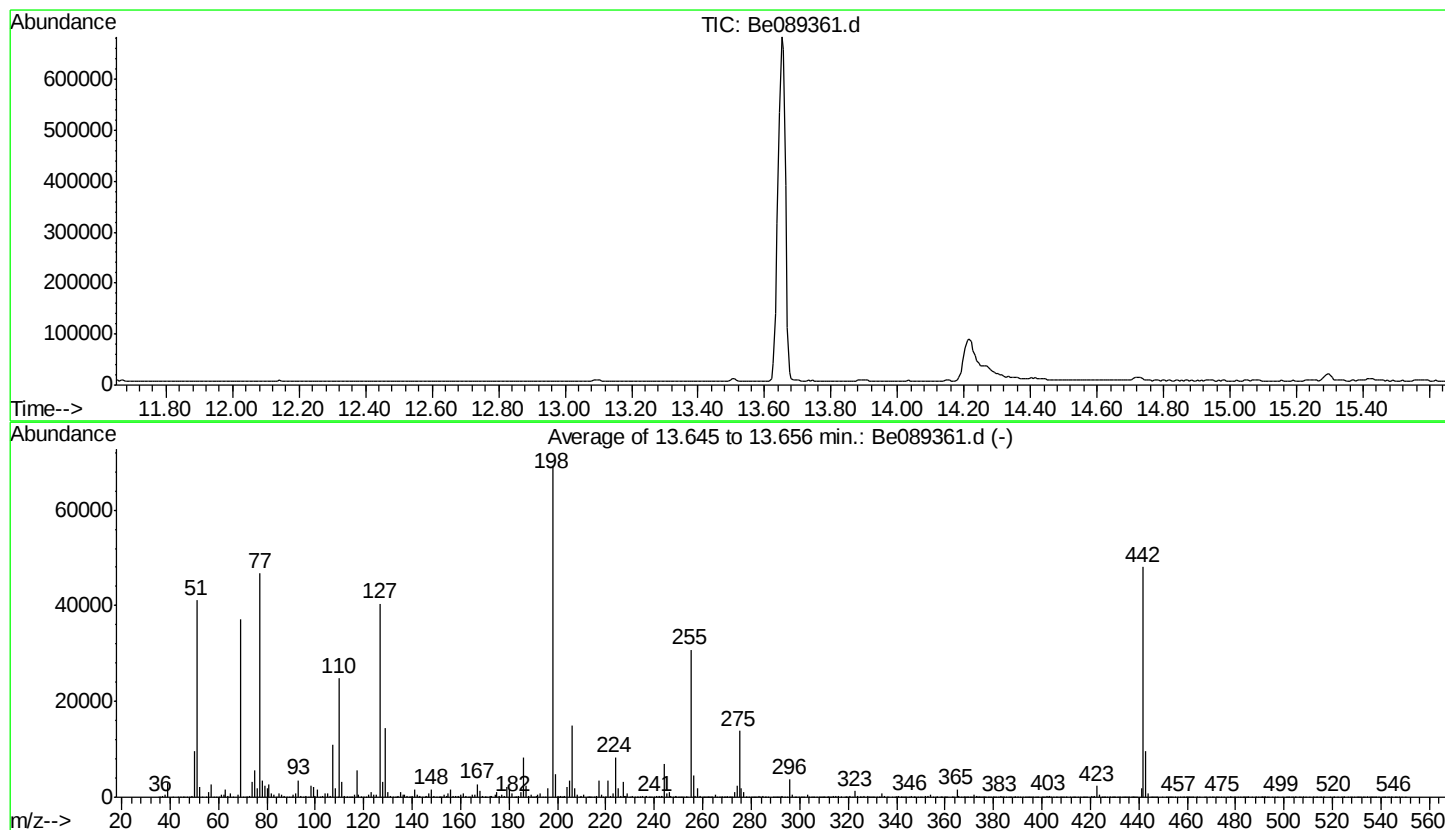

AutoFind: Scans 2086, 2087, 2088; Background Corrected with Scan 2077

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.3	41095	PASS
68	69	0.00	2	1.5	562	PASS
69	198	0.00	100	53.6	37140	PASS
70	69	0.00	2	0.3	129	PASS
127	198	10	80	58.4	40480	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	69258	PASS
199	198	5	9	6.9	4763	PASS
275	198	10	60	20.0	13820	PASS
365	198	1	100	2.3	1568	PASS
441	443	0.01	100	19.5	1870	PASS
442	198	50	100	69.5	48116	PASS
443	442	15	24	19.9	9572	PASS