

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010815\
 Data File : BE089375.D
 Acq On : 8 Jan 2015 20:28
 Operator : TP/IZ
 Sample : F5245-20RX
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Y9RC5

Quant Time: Jan 09 12:11:55 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 09 01:27:36 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1182	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	4661	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.65	164	2473	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	3725	0.40	ng/ul	0.00
18) Chrysene-d12	18.07	240	2573	0.40	ng/ul	0.00
22) Perylene-d12	21.12	264	2236	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.11	96	488	0.27	ng/uL	0.00
6) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
						Qvalue
17) Fluoranthene	14.96	202	1042	0.03	ng/ul#	60
19) Pyrene	15.40	202	1133	0.03	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010815\
Data File : BE089375.D
Acq On : 8 Jan 2015 20:28
Operator : TP/IZ
Sample : F5245-20RX
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Y9RC5

Quant Time: Jan 09 12:11:55 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 09 01:27:36 2015
Response via : Initial Calibration




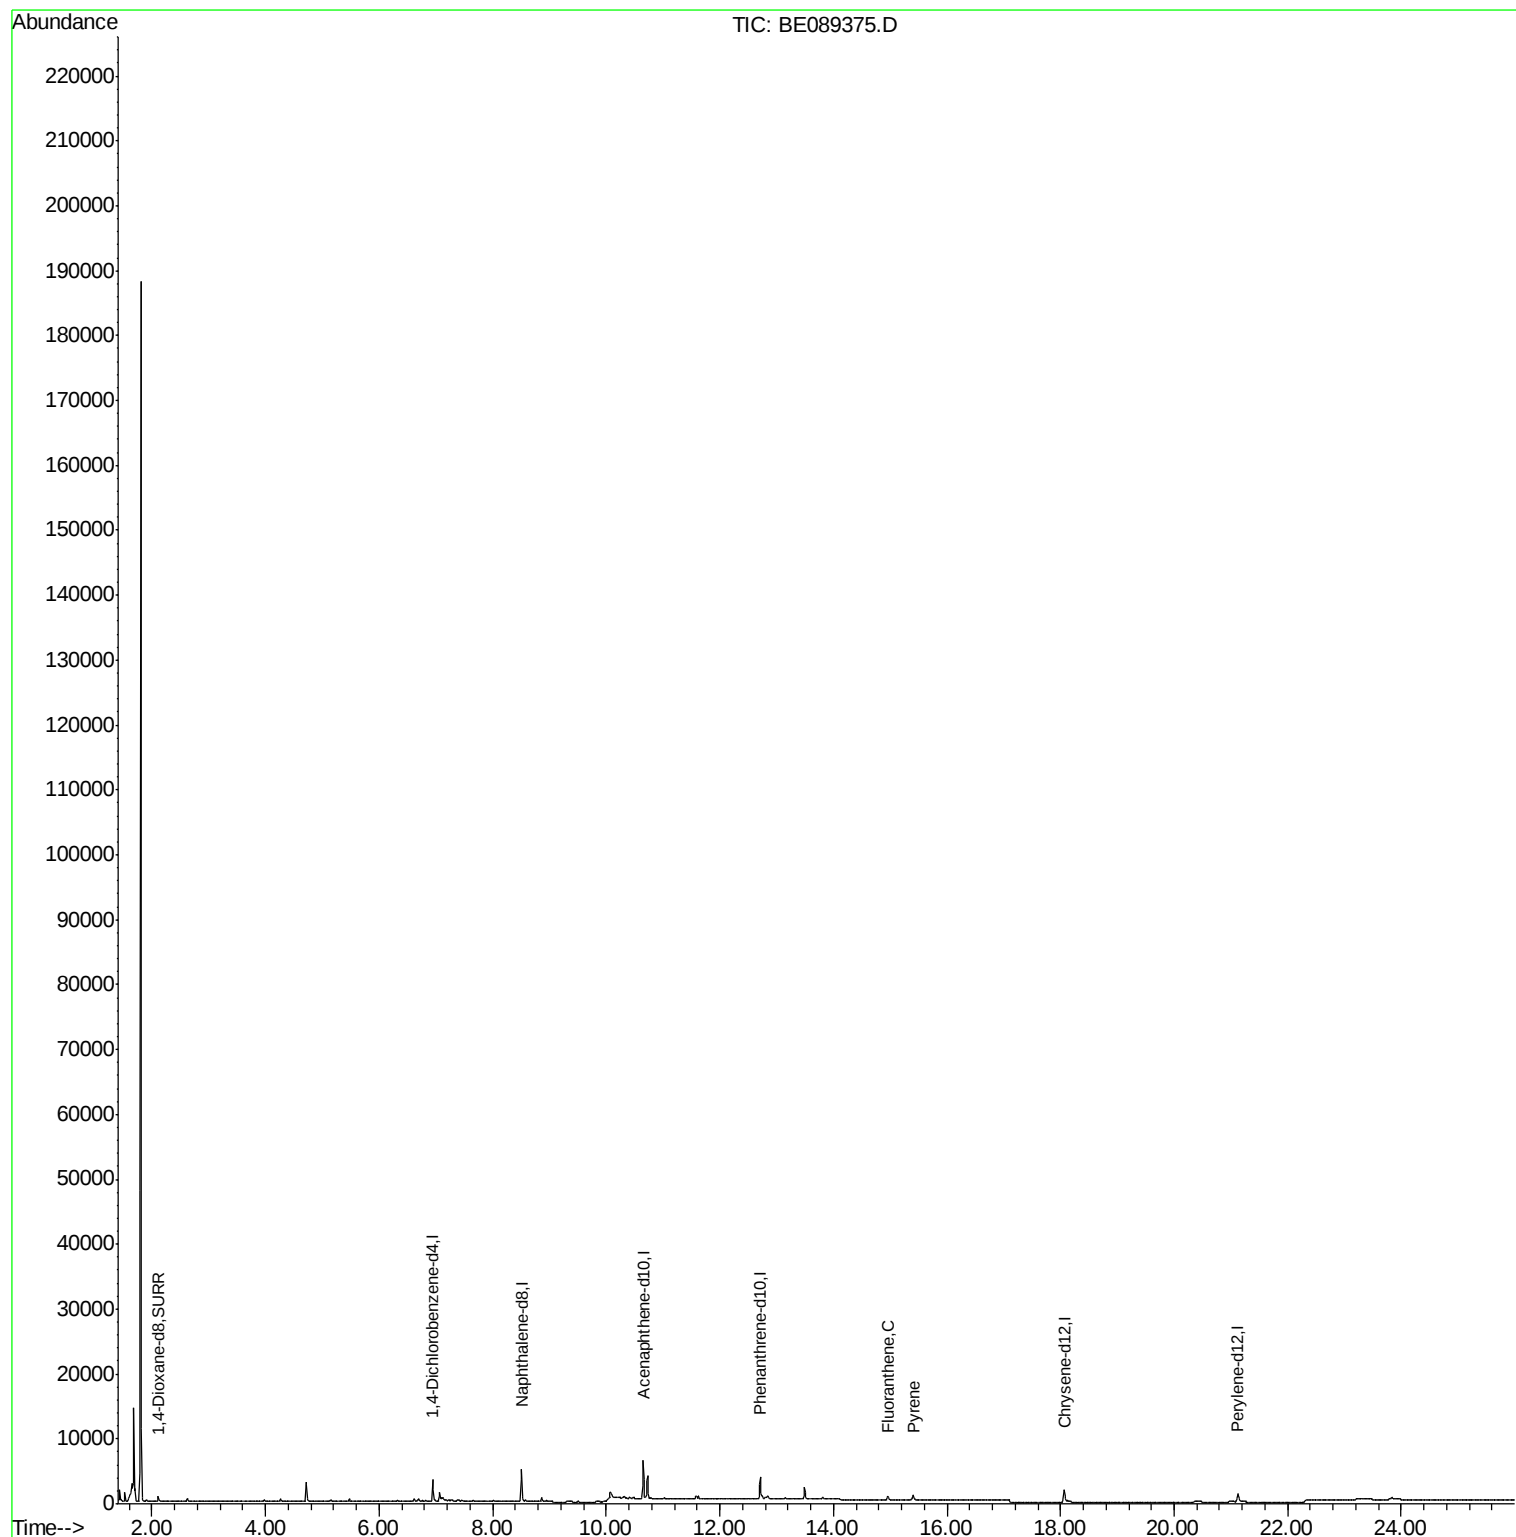


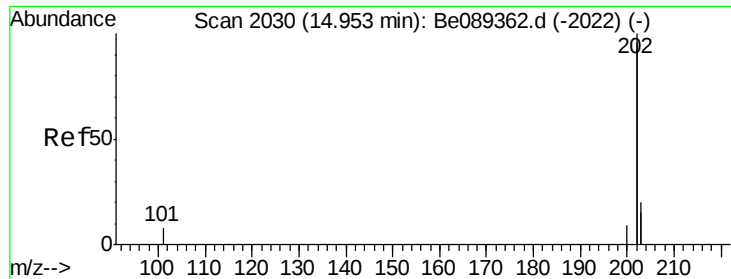

#17
Fluoranthene
 Concen: 0.03 ng/ul
 RT: 14.96 min Scan# 2031
 Delta R.T. 0.01 min
 Lab File: BE089375.D
 Acq: 8 Jan 2015 20:28

Instrument :
 BNA_E
 ClientSampleId :
 Y9RC5

Tgt Ion:202 Resp: 1042
 Ion Ratio Lower Upper
 202 100
 101 9.7 0.0 24.6
 203 38.3 0.0 37.8#

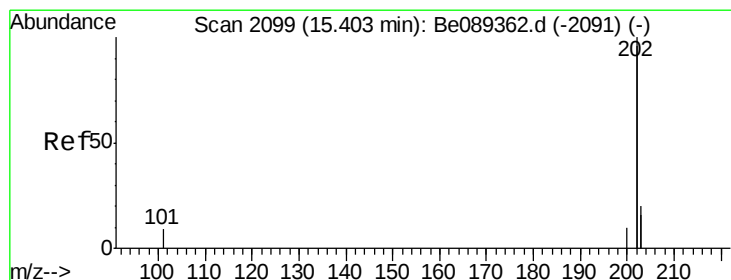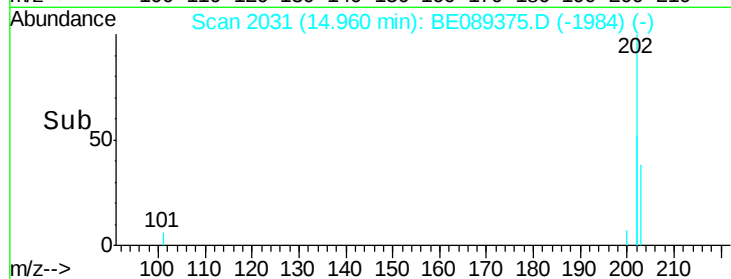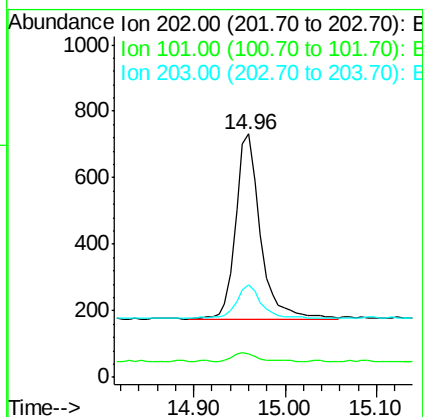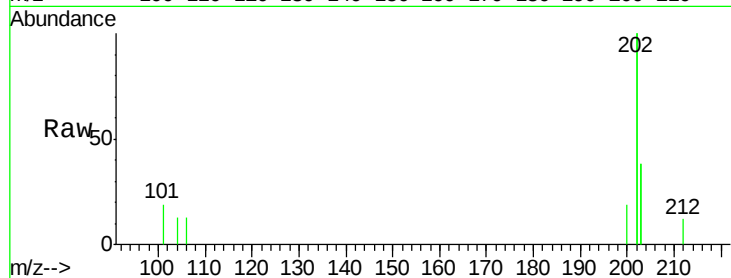

#19
Pyrene
 Concen: 0.03 ng/ul
 RT: 15.40 min Scan# 2099
 Delta R.T. 0.00 min
 Lab File: BE089375.D
 Acq: 8 Jan 2015 20:28

Tgt Ion:202 Resp: 1133
 Ion Ratio Lower Upper
 202 100
 200 9.6 4.2 6.4#
 203 37.1 14.4 21.6#

