


1,4-Dioxane

Response Ratio

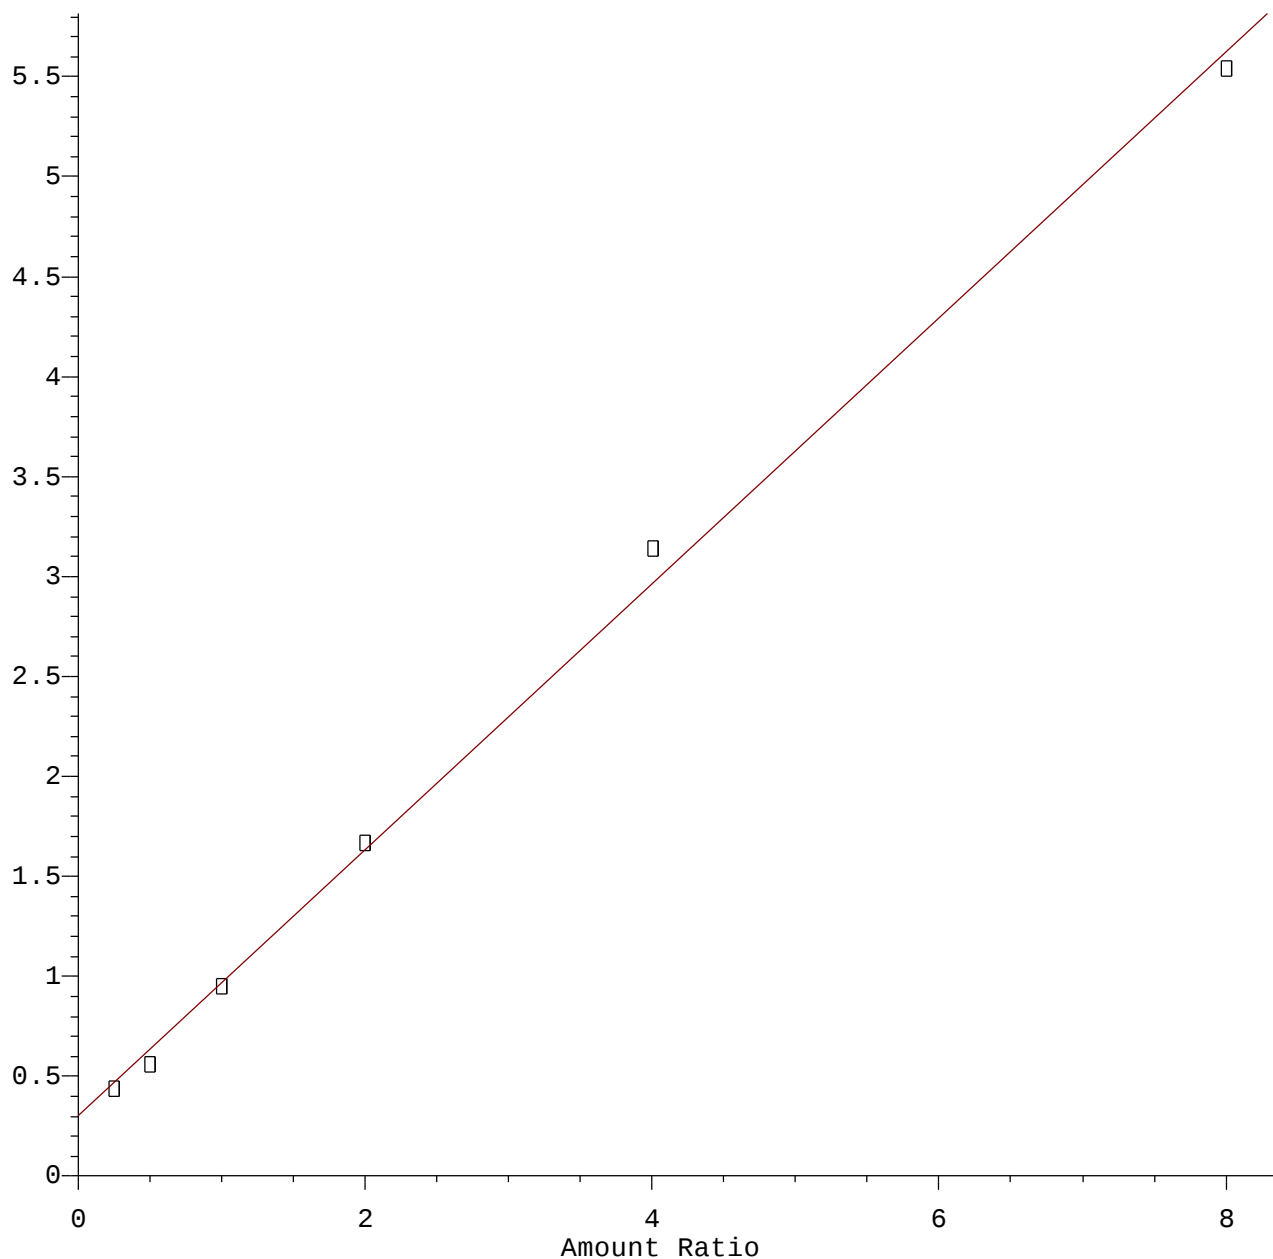


Resp Ratio = 6.66e-001 * Amt + 2.99e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
Calibration Table Last Updated: Wed Jan 08 18:36:25 2020

Pentachlorophenol

Response Ratio

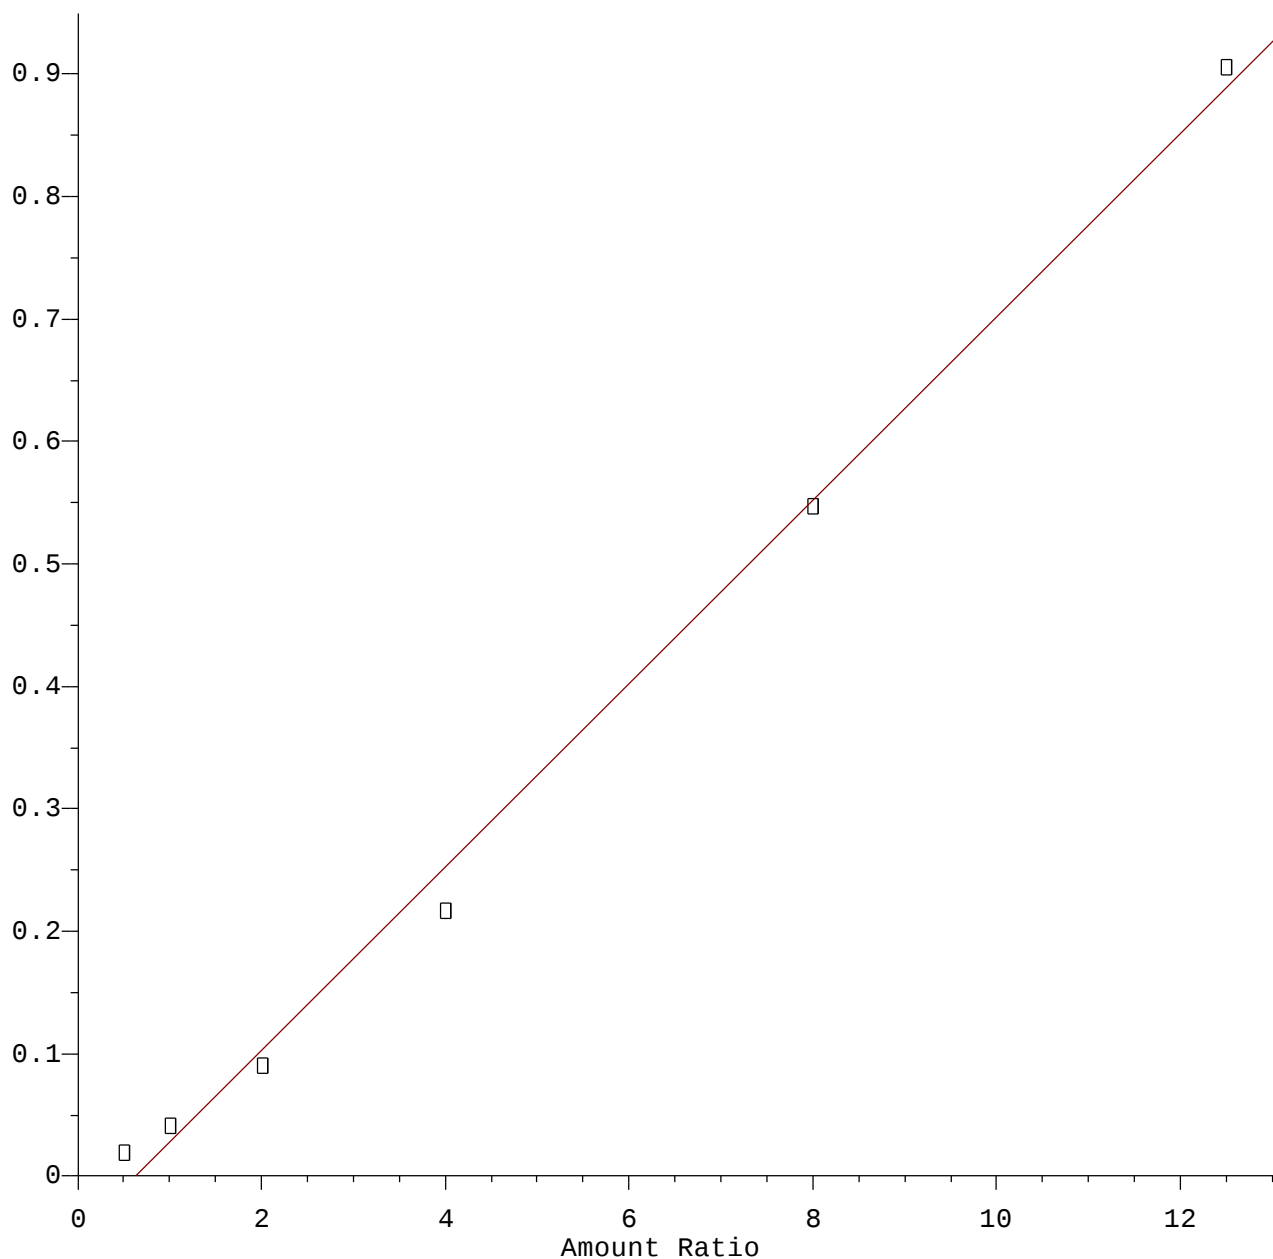


Resp Ratio = $7.49 \times 10^{-2} \times \text{Amt} - 4.68 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
Calibration Table Last Updated: Wed Jan 08 18:36:25 2020

Pentachlorophenol

Response Ratio

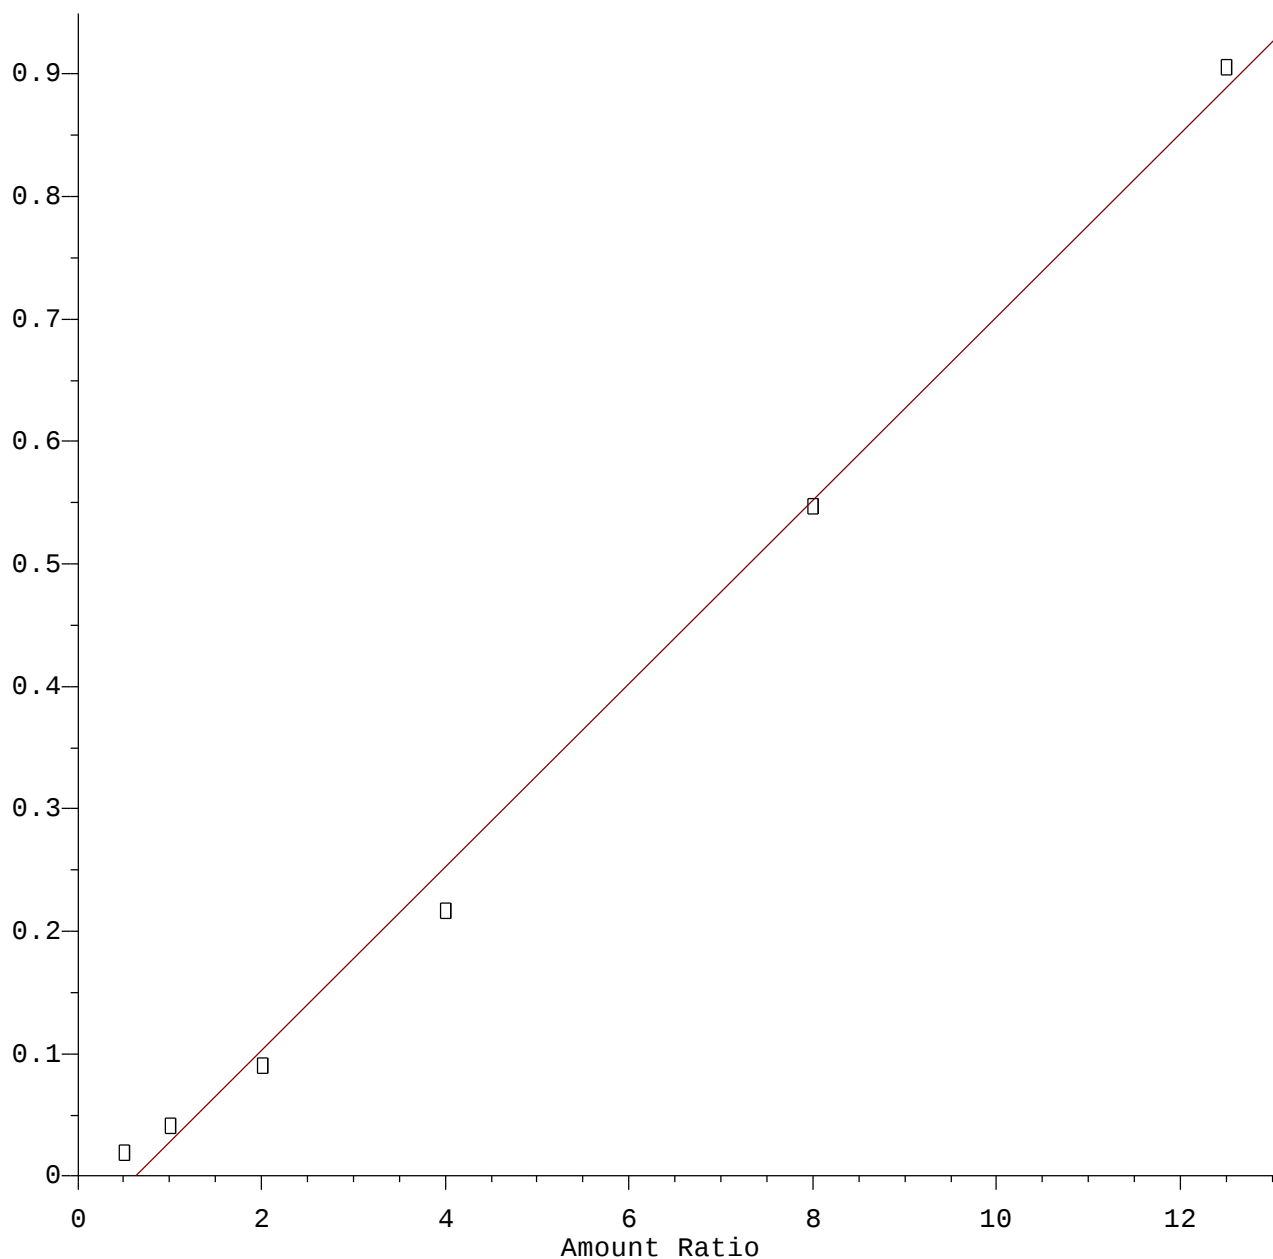

Resp Ratio = $7.49 \times 10^{-2} \times \text{Amt} - 4.68 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
Calibration Table Last Updated: Wed Jan 08 18:36:25 2020