


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE010820\
Data File : BE101000.D
Acq On : 8 Jan 2020 12:39
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 08 18:36:25 2020

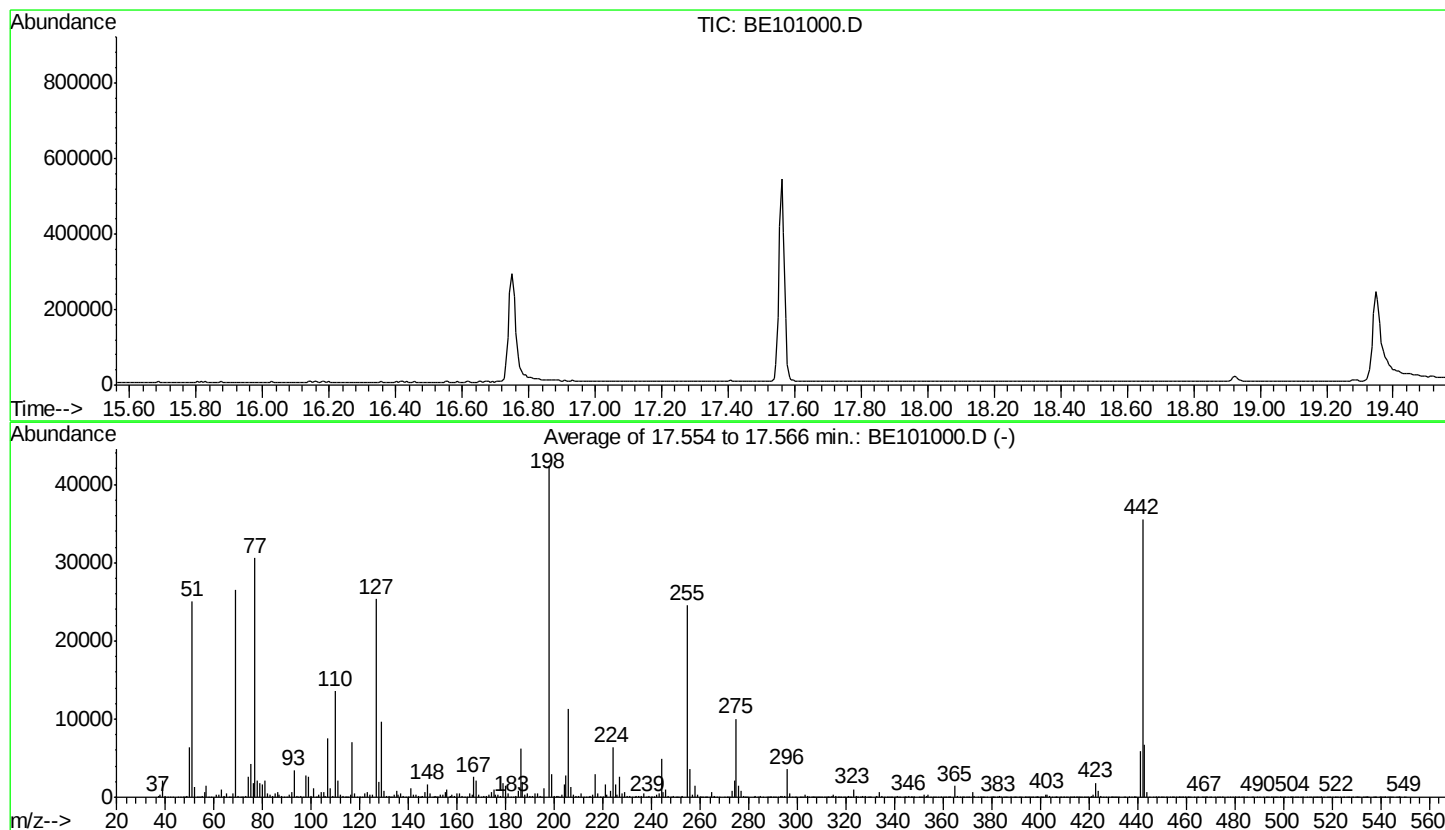

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2540

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.0	25005	PASS
68	69	0.00	2	1.9	493	PASS
69	198	0.00	100	62.7	26577	PASS
70	69	0.00	2	0.6	161	PASS
127	198	10	80	59.8	25353	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42402	PASS
199	198	5	9	6.8	2872	PASS
275	198	10	60	23.7	10041	PASS
365	198	1	100	3.4	1431	PASS
441	198	0.01	100	13.8	5855	PASS
442	198	50	100	83.7	35482	PASS
443	442	15	24	19.1	6788	PASS