


Data Path : Z:\HPCHEM1\BNA_E\Data\BE010915\
 Data File : BE089377.D
 Acq On : 9 Jan 2015 10:31
 Operator : TP/IZ
 Sample : DFTPP38
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP38

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM010715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 08 10:41:47 2015

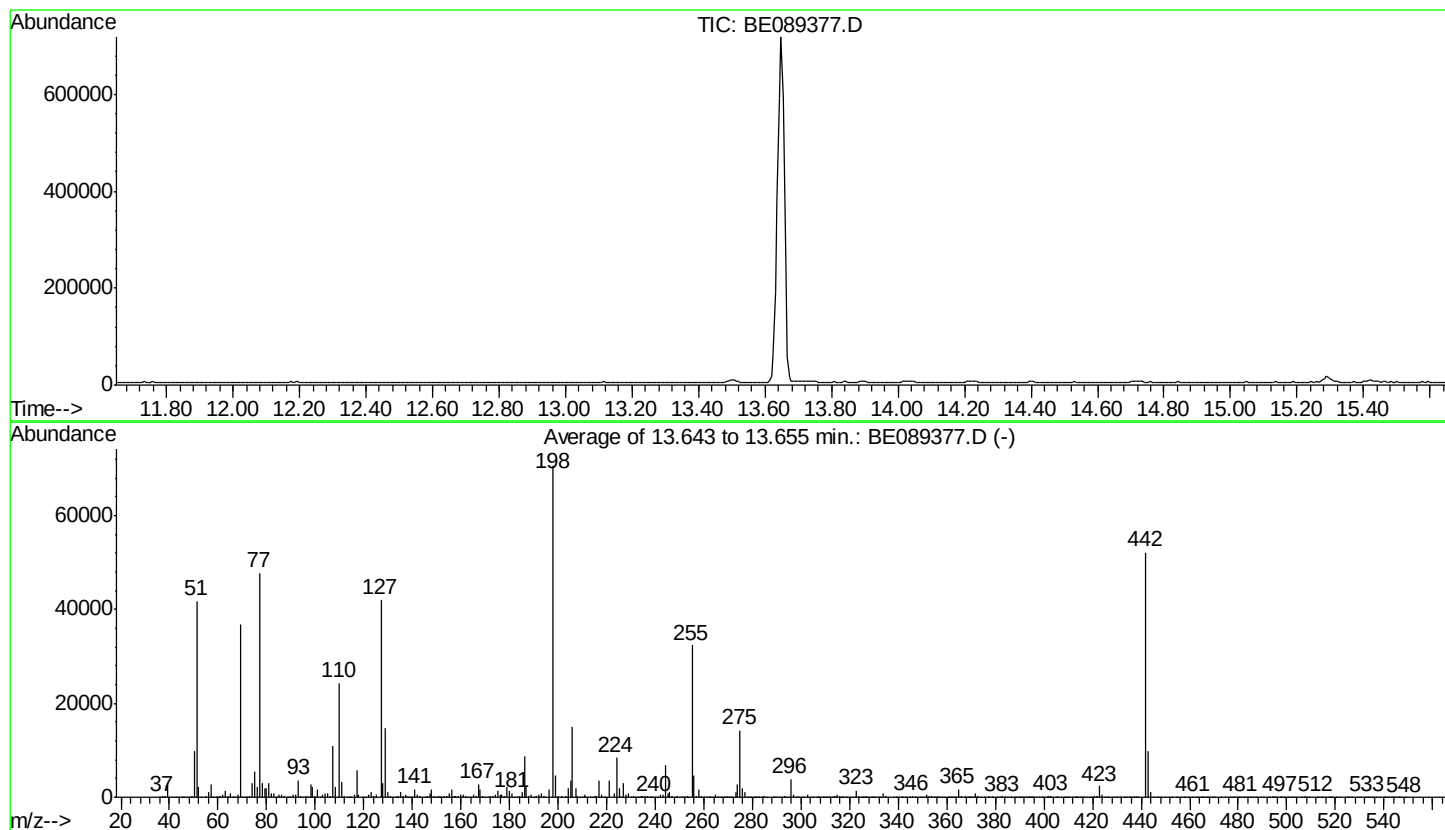

AutoFind: Scans 2086, 2087, 2088; Background Corrected with Scan 2077

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.1	41750	PASS
68	69	0.00	2	1.2	434	PASS
69	198	0.00	100	52.1	36823	PASS
70	69	0.00	2	0.4	144	PASS
127	198	10	80	59.5	42071	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	70679	PASS
199	198	5	9	6.6	4673	PASS
275	198	10	60	20.3	14323	PASS
365	198	1	100	2.3	1647	PASS
441	443	0.01	100	0.0	0	FAIL *
442	198	50	100	73.8	52146	PASS
443	442	15	24	18.7	9736	PASS