

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010915\
 Data File : BE089379.D
 Acq On : 9 Jan 2015 11:42
 Operator : TP/IZ
 Sample : G1029-01RX
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Y9R90RX

Quant Time: Jan 12 09:44:46 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 09 23:22:39 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1195	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	4820	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.65	164	2516	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	3925	0.40	ng/ul	0.00
18) Chrysene-d12	18.07	240	2737	0.40	ng/ul	0.00
22) Perylene-d12	21.12	264	2391	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.11	96	477	0.27	ng/uL	0.00
6) 2-Methylnaphthalene-d10	0.00	152	0	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
17) Fluoranthene	14.99	202	1158	0.03	ng/ul	Qvalue 67
19) Pyrene	15.41	202	1353	0.04	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010915\
Data File : BE089379.D
Acq On : 9 Jan 2015 11:42
Operator : TP/IZ
Sample : G1029-01RX
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Y9R90RX

Quant Time: Jan 12 09:44:46 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 09 23:22:39 2015
Response via : Initial Calibration




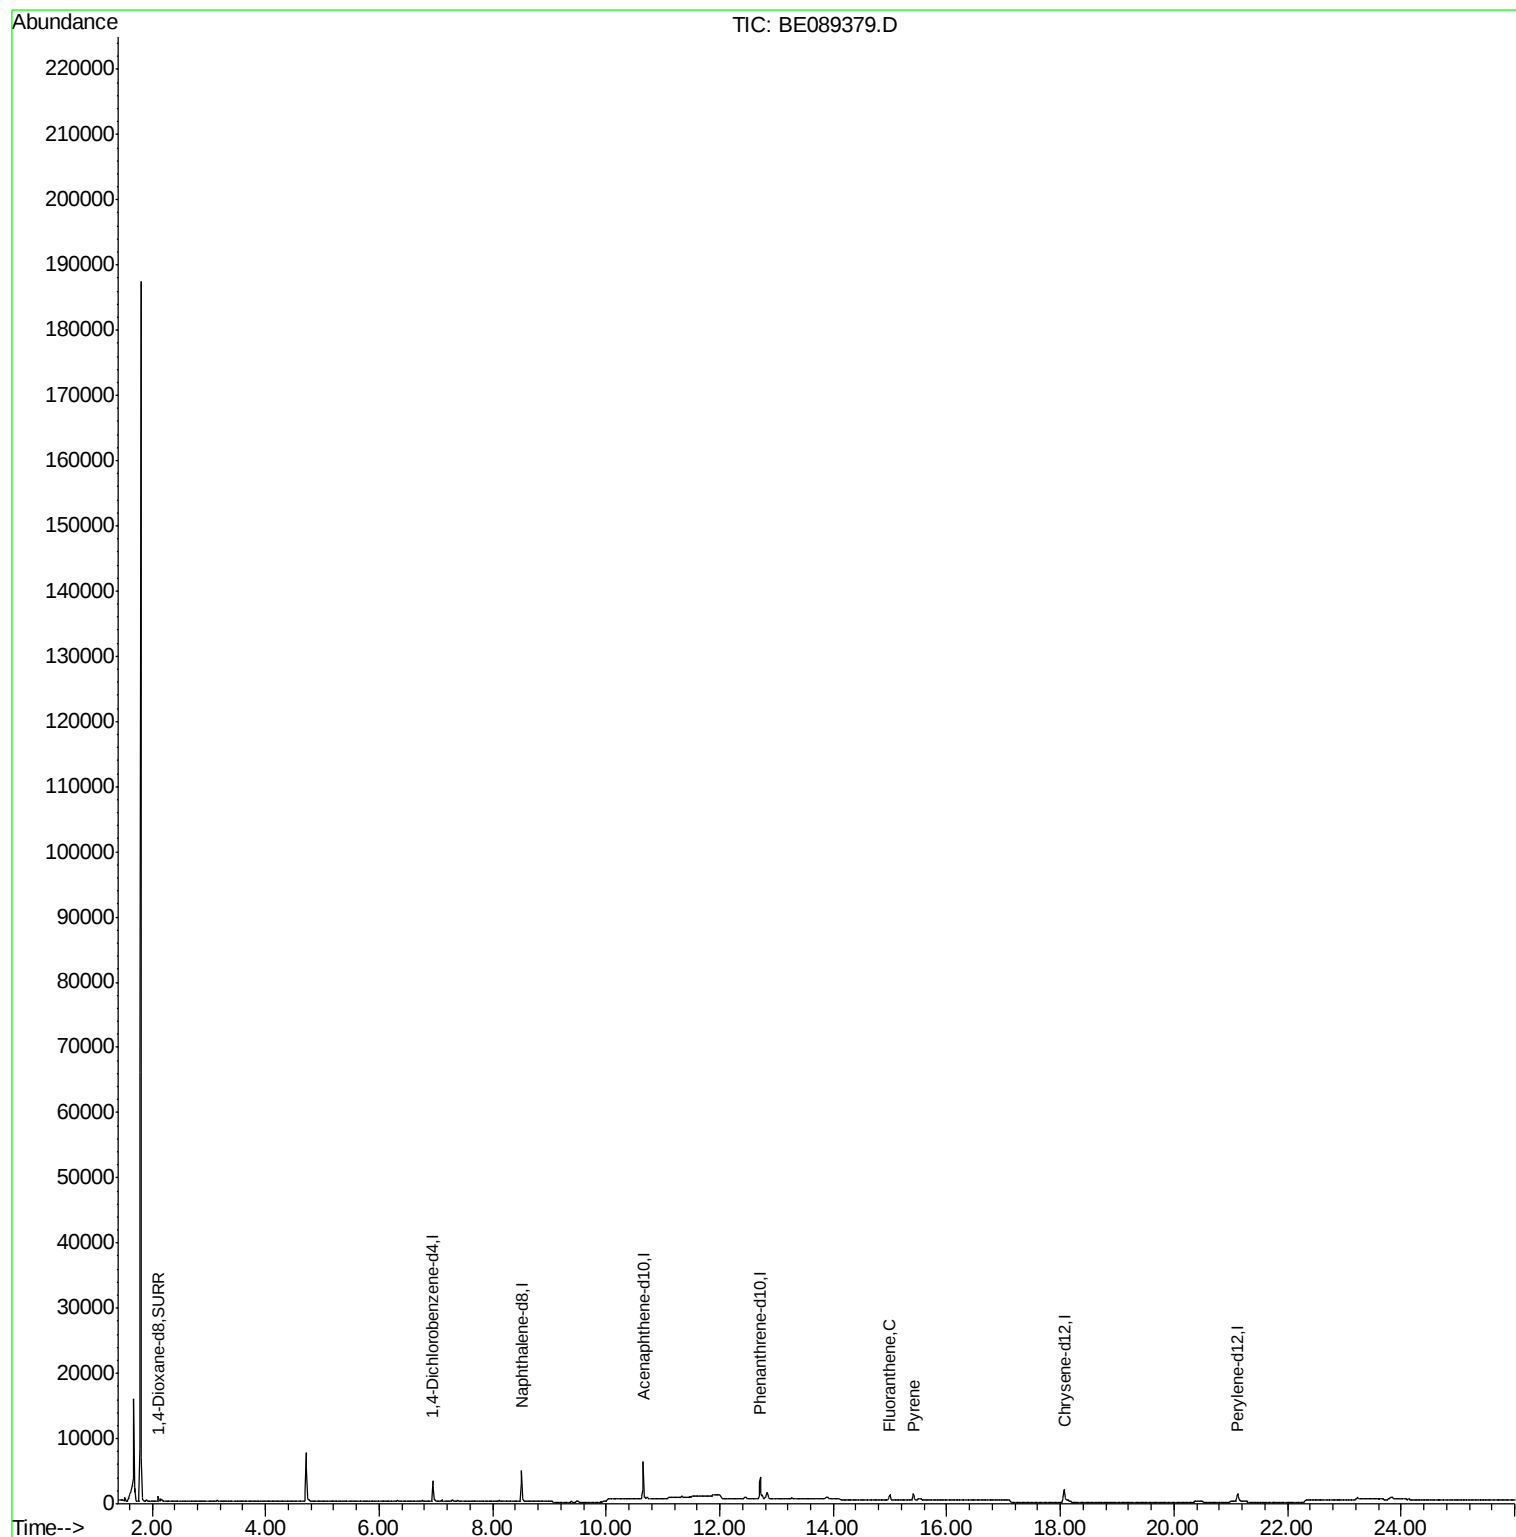


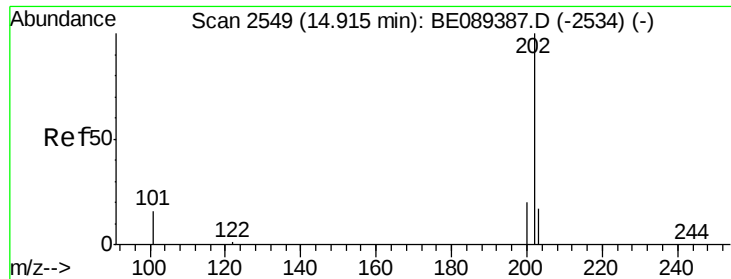

#17
Fluoranthene
 Concen: 0.03 ng/ul
 RT: 14.99 min Scan# 2035
 Delta R.T. 0.00 min
 Lab File: BE089379.D
 Acq: 9 Jan 2015 11:42

Instrument :
 BNA_E
 ClientSampleId :
 Y9R90RX

Tgt Ion:202 Resp: 1158
 Ion Ratio Lower Upper
 202 100
 101 9.5 0.0 24.6
 203 34.6 0.0 37.8

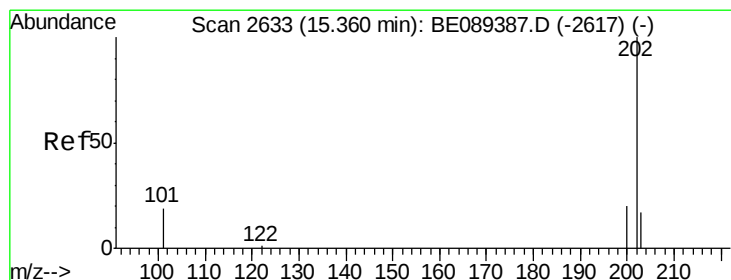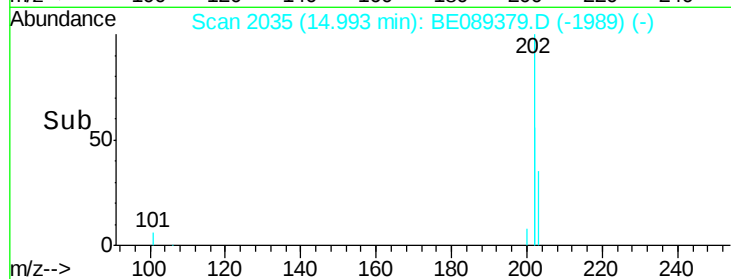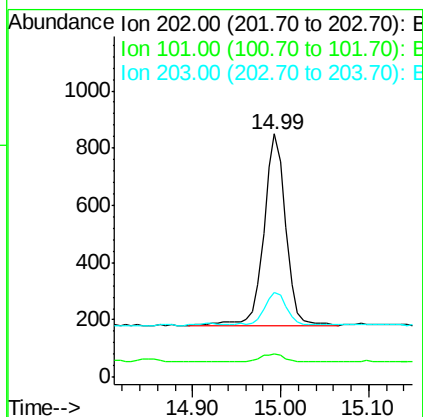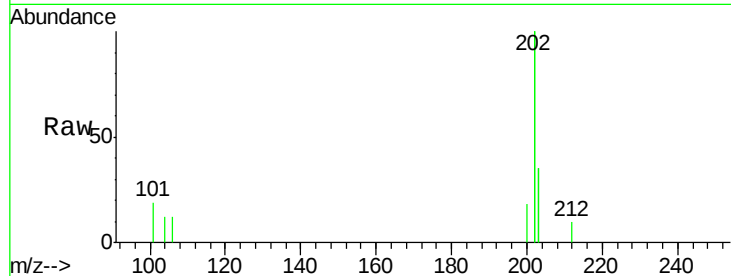

#19
Pyrene
 Concen: 0.04 ng/ul
 RT: 15.41 min Scan# 2099
 Delta R.T. 0.00 min
 Lab File: BE089379.D
 Acq: 9 Jan 2015 11:42

Tgt Ion:202 Resp: 1353
 Ion Ratio Lower Upper
 202 100
 200 8.9 4.2 6.4#
 203 33.4 14.4 21.6#

