

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010915\
 Data File : BE089380.D
 Acq On : 9 Jan 2015 12:15
 Operator : TP/IZ
 Sample : G1029-02RX
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Y9R91RX

Quant Time: Jan 12 09:54:46 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 09 23:24:59 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1427	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	5738	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.65	164	2898	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	4383	0.40	ng/ul	0.00
18) Chrysene-d12	18.07	240	2877	0.40	ng/ul	0.00
22) Perylene-d12	21.12	264	2436	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.12	96	542	0.25	ng/uL	0.00
6) 2-Methylnaphthalene-d10	0.00	152	0	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
17) Fluoranthene	14.96	202	1473	0.04	ng/ul	Qvalue 71
19) Pyrene	15.41	202	1591	0.04	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010915\
Data File : BE089380.D
Acq On : 9 Jan 2015 12:15
Operator : TP/IZ
Sample : G1029-02RX
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Y9R91RX

Quant Time: Jan 12 09:54:46 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 09 23:24:59 2015
Response via : Initial Calibration

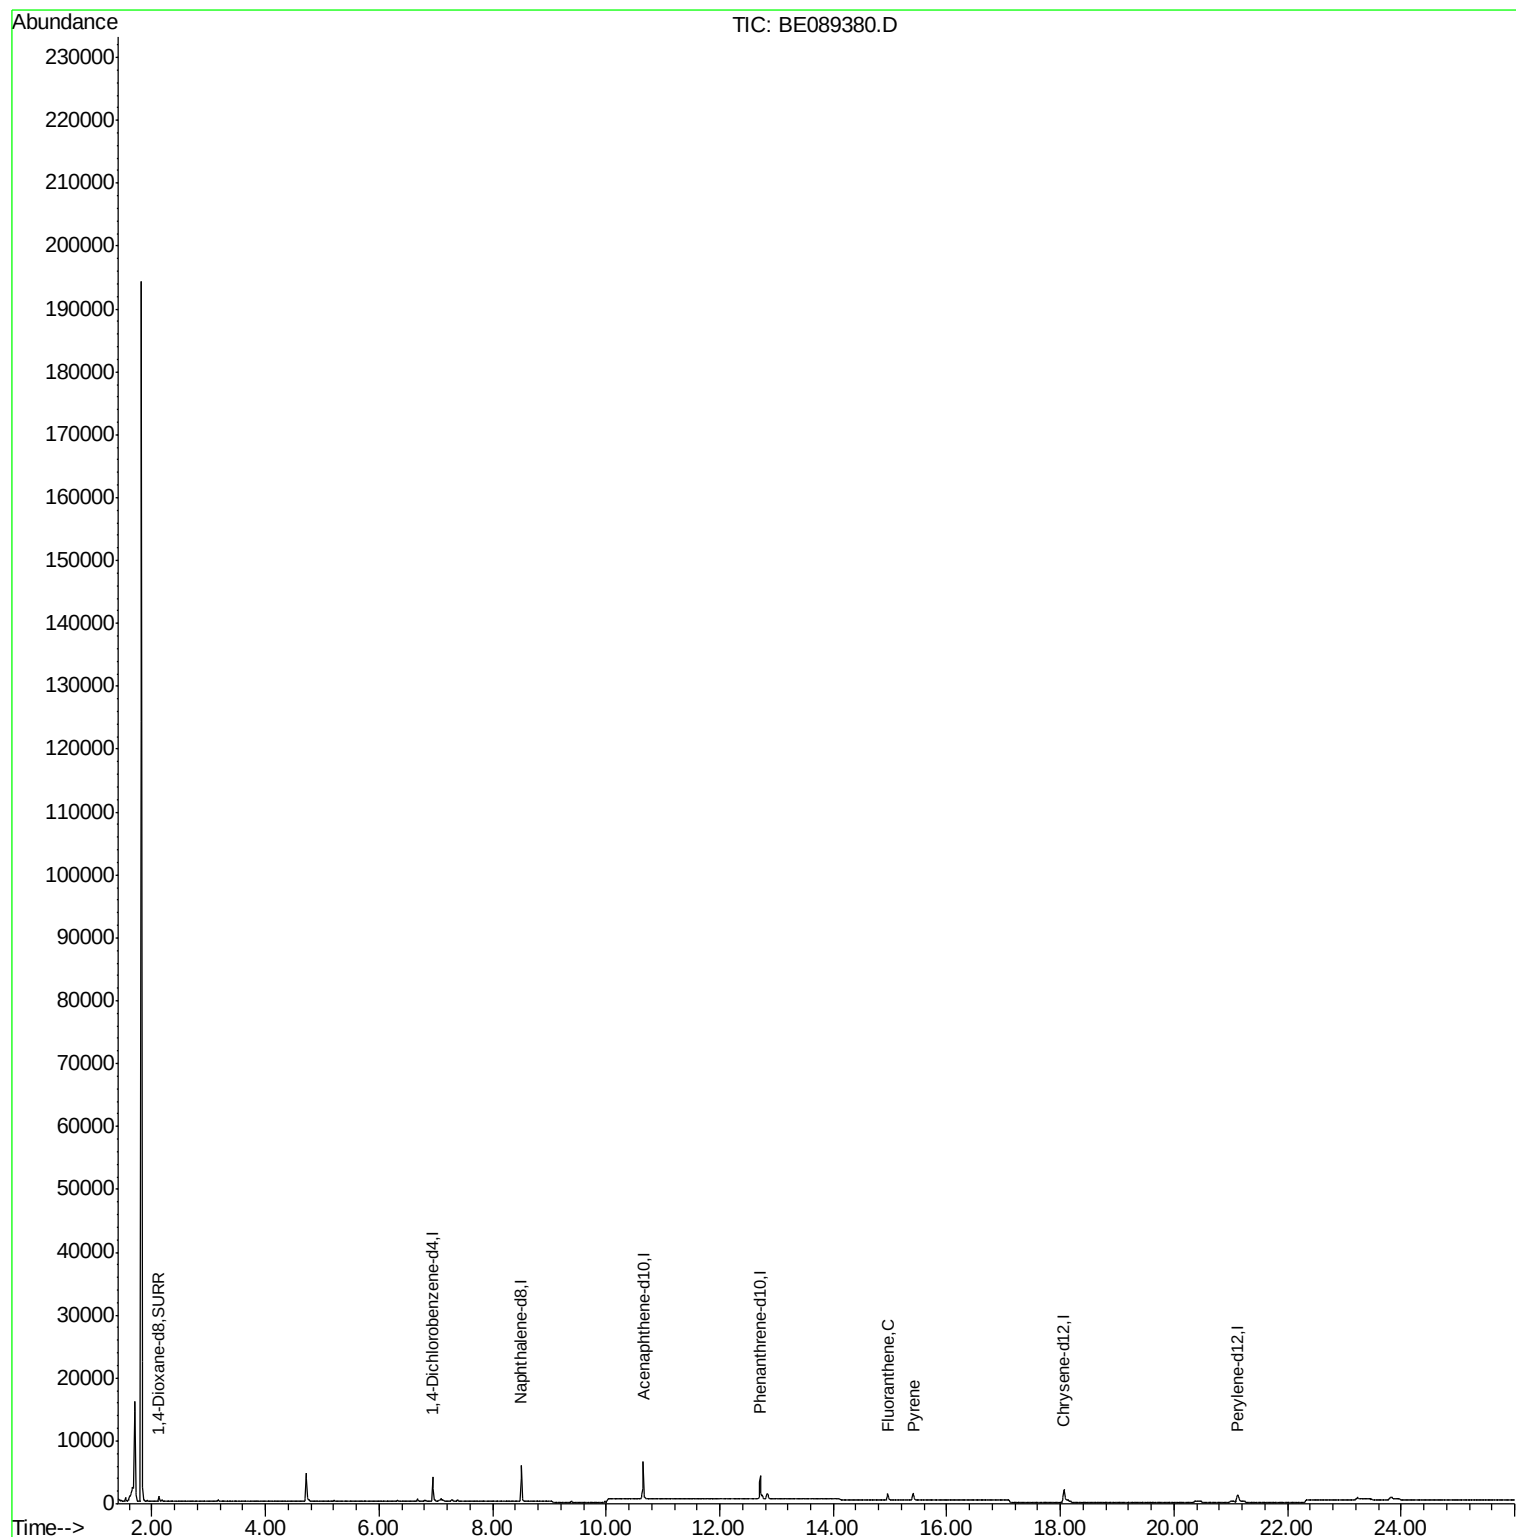

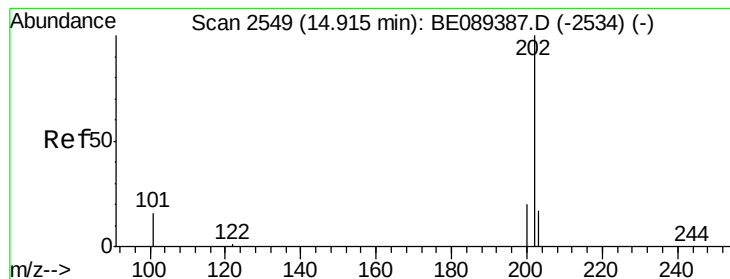

#17

Fluoranthene

Concen: 0.04 ng/ul

RT: 14.96 min Scan# 2030

Delta R.T. 0.00 min

Lab File: BE089380.D

Acq: 9 Jan 2015 12:15

Instrument :

BNA_E

ClientSampleId :

Y9R91RX


Tgt Ion:202 Resp: 1473

Ion Ratio Lower Upper

202 100

101 8.1 0.0 24.6




203 32.8 0.0 37.8

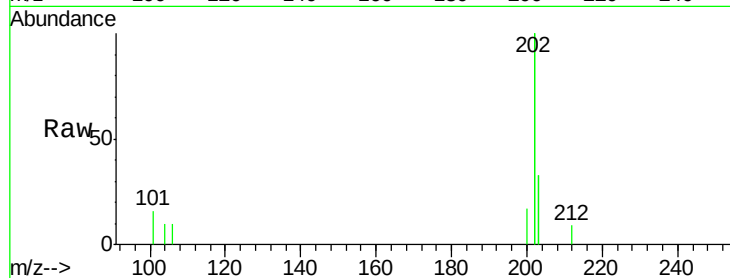

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

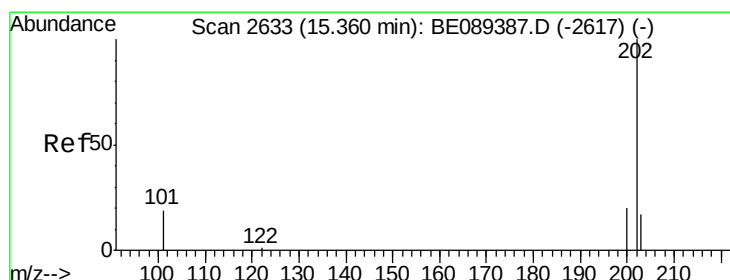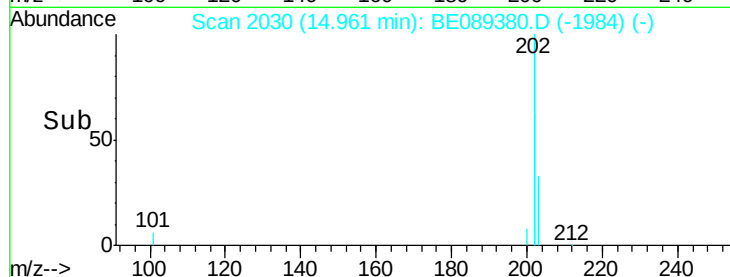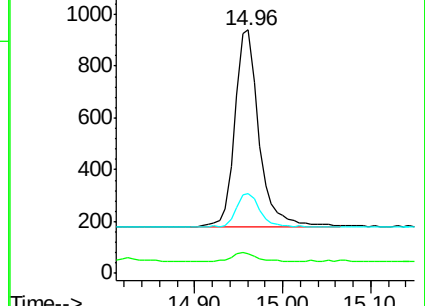

#19

Pyrene

Concen: 0.04 ng/ul

RT: 15.41 min Scan# 2099

Delta R.T. 0.00 min

Lab File: BE089380.D

Acq: 9 Jan 2015 12:15


Tgt Ion:202 Resp: 1591

Ion Ratio Lower Upper

202 100

200 8.5 4.2 6.4#

203 33.4 14.4 21.6#

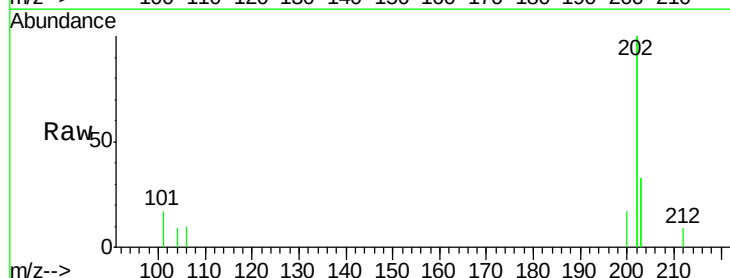

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

