

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010915\
 Data File : BE089383.D
 Acq On : 9 Jan 2015 14:35
 Operator : TP/IZ
 Sample : G1029-04RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 Y9RA6RX

Quant Time: Jan 12 09:59:35 2015
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 09 23:27:44 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	1294	0.40	ng/ul	0.00
4) Naphthalene-d8	8.51	136	5218	0.40	ng/ul	0.00
8) Acenaphthene-d10	10.65	164	2637	0.40	ng/ul	0.00
12) Phenanthrene-d10	12.71	188	4028	0.40	ng/ul	0.00
18) Chrysene-d12	18.07	240	2753	0.40	ng/ul	0.00
22) Perylene-d12	21.13	264	2281	0.40	ng/ul	0.00
System Monitoring Compounds						
2) 1,4-Dioxane-d8	2.12	96	453	0.23	ng/uL	0.01
6) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul	
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul	
Target Compounds						
17) Fluoranthene	14.96	202	2027	0.05	ng/ul	Qvalue 75
19) Pyrene	15.41	202	2108	0.06	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010915\
Data File : BE089383.D
Acq On : 9 Jan 2015 14:35
Operator : TP/IZ
Sample : G1029-04RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
Y9RA6RX

Quant Time: Jan 12 09:59:35 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM01.2-EPA-SIM-BE123014.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 09 23:27:44 2015
Response via : Initial Calibration




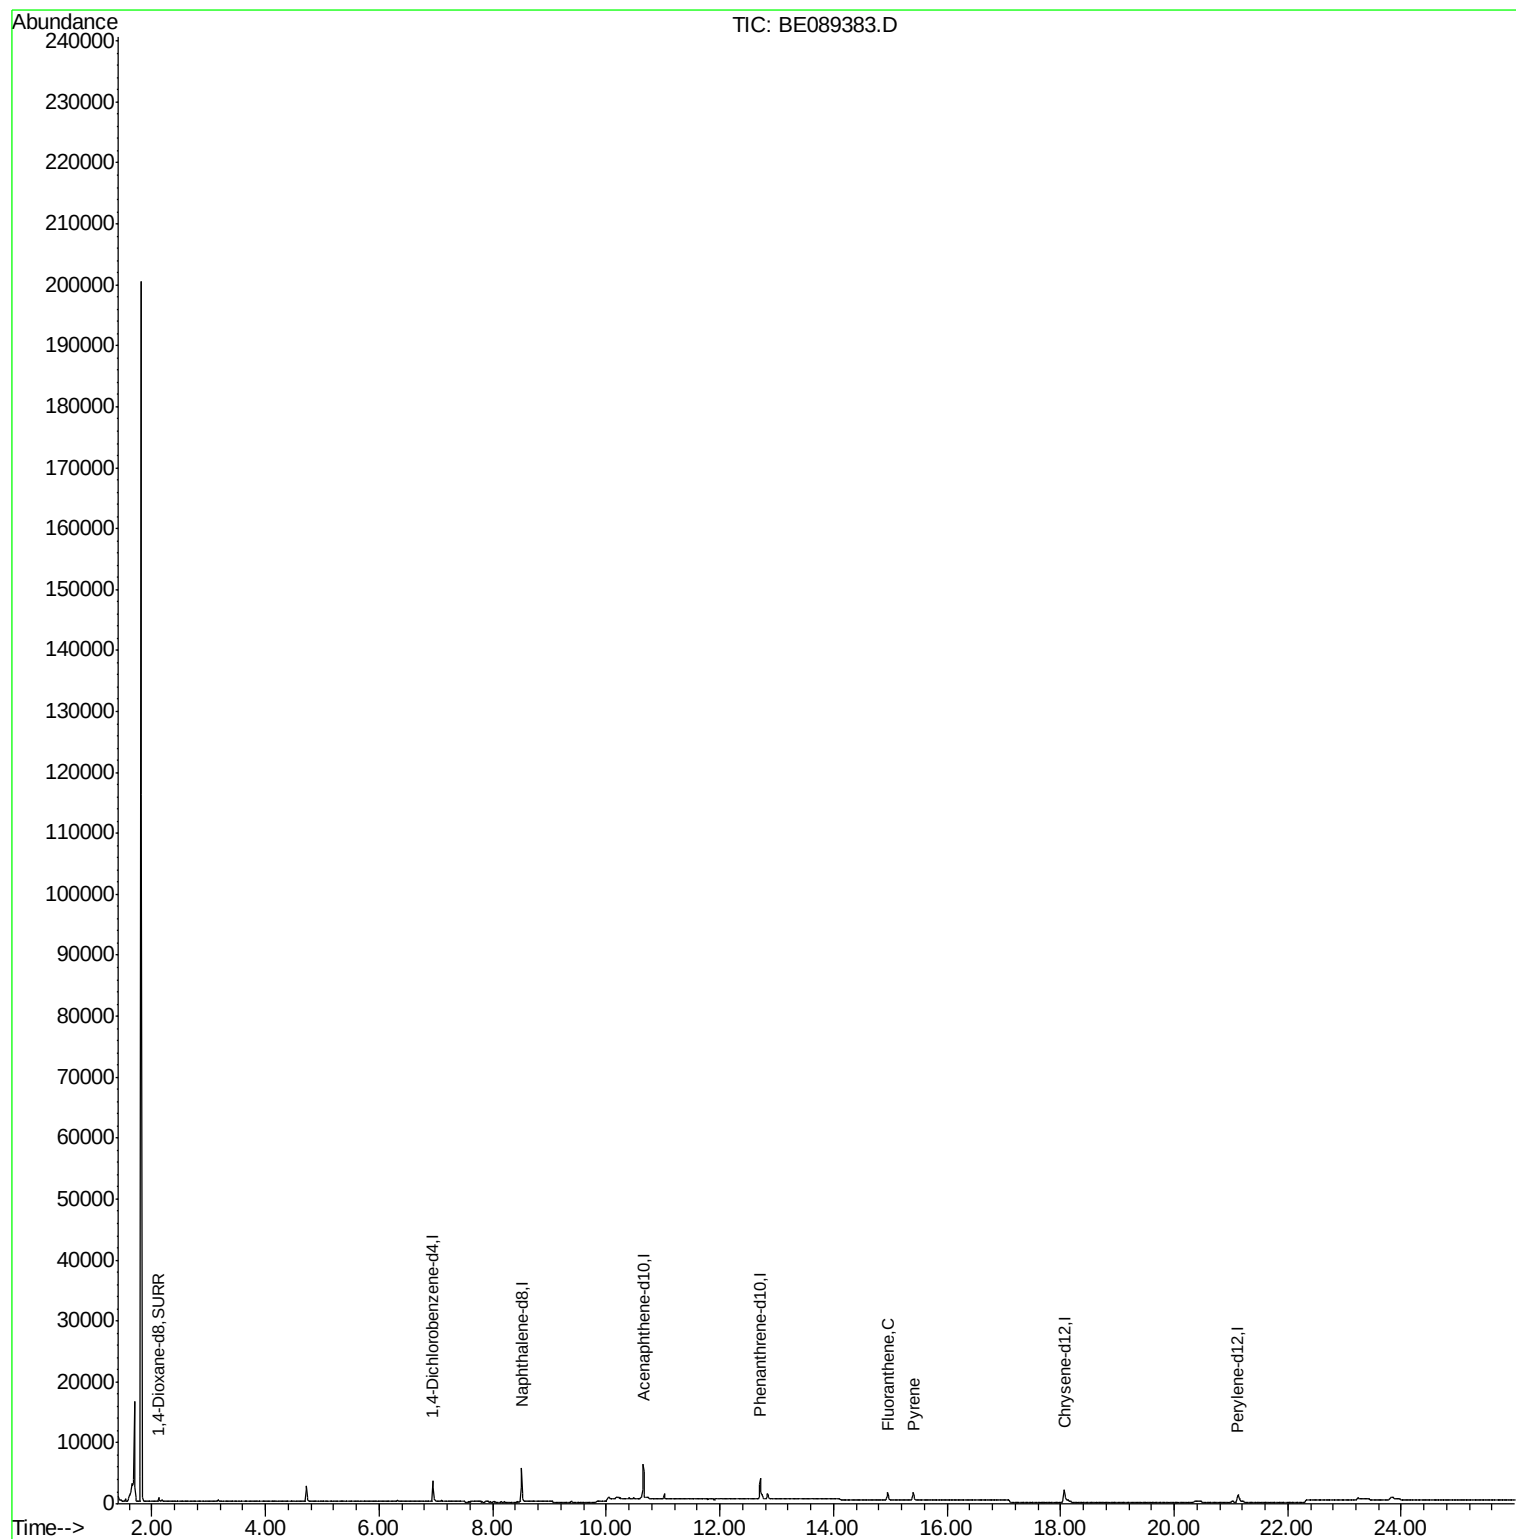


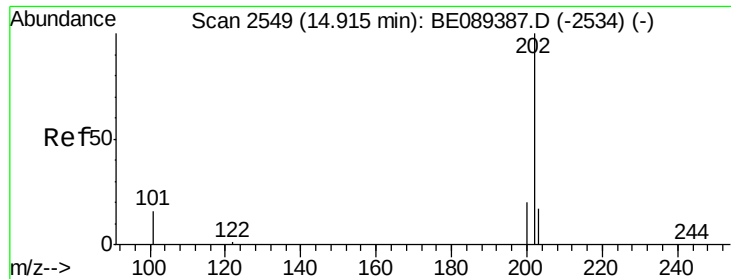

#17
 Fluoranthene
 Concen: 0.05 ng/ul
 RT: 14.96 min Scan# 2031
 Delta R.T. 0.01 min
 Lab File: BE089383.D
 Acq: 9 Jan 2015 14:35

Instrument :
 BNA_E
 ClientSampleId :
 Y9RA6RX

Tgt Ion:202 Resp: 2027
 Ion Ratio Lower Upper
 202 100
 101 7.4 0.0 24.6
 203 30.7 0.0 37.8

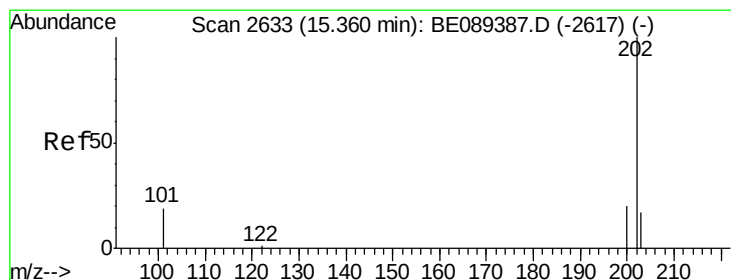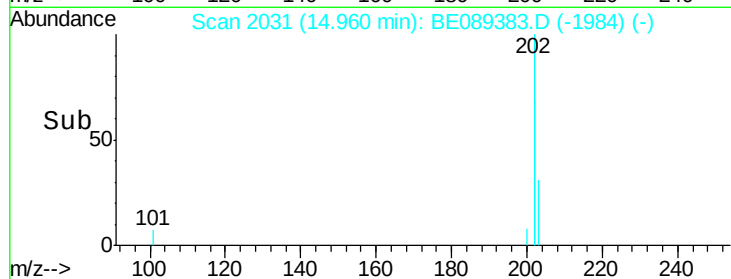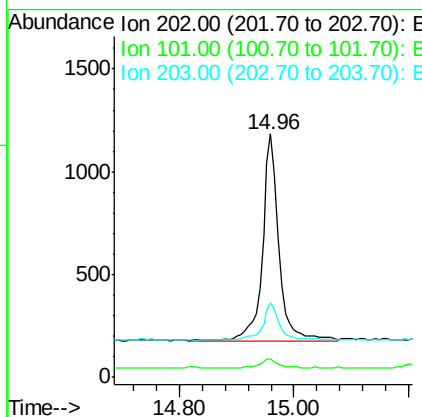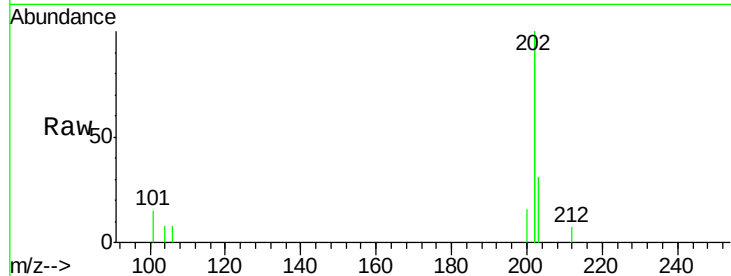

#19
 Pyrene
 Concen: 0.06 ng/ul
 RT: 15.41 min Scan# 2100
 Delta R.T. 0.01 min
 Lab File: BE089383.D
 Acq: 9 Jan 2015 14:35

Tgt Ion:202 Resp: 2108
 Ion Ratio Lower Upper
 202 100
 200 7.8 4.2 6.4#
 203 30.1 14.4 21.6#

