


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE010915\
 Data File : BE089386.D
 Acq On : 9 Jan 2015 17:19
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-PAH-BASE-BE010715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 08 15:21:44 2015

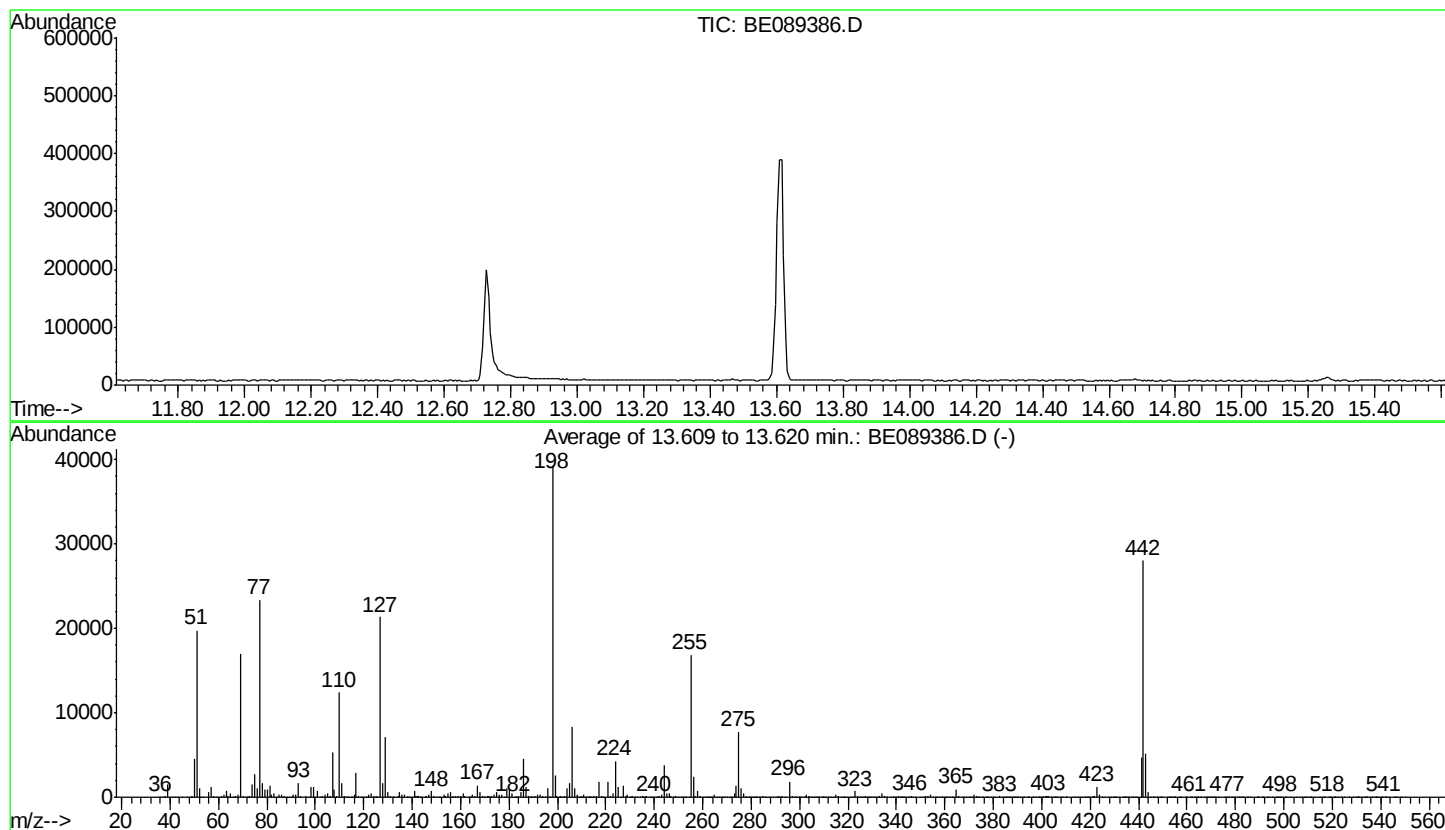

AutoFind: Scans 2080, 2081, 2082; Background Corrected with Scan 2070

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.2	19716	PASS
68	69	0.00	2	1.7	282	PASS
69	198	0.00	100	43.4	17055	PASS
70	69	0.00	2	0.7	111	PASS
127	198	10	80	54.4	21350	PASS
197	198	0.00	2	0.1	41	PASS
198	198	100	100	100.0	39273	PASS
199	198	5	9	6.6	2595	PASS
275	198	10	60	19.8	7782	PASS
365	198	1	100	2.3	910	PASS
441	442	0.01	24	16.8	4696	PASS
442	198	50	100	71.3	27997	PASS
443	442	15	24	18.2	5098	PASS