


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE011018\
Data File : BE095064.D
Acq On : 10 Jan 2018 9:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121417.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 27 12:15:11 2017

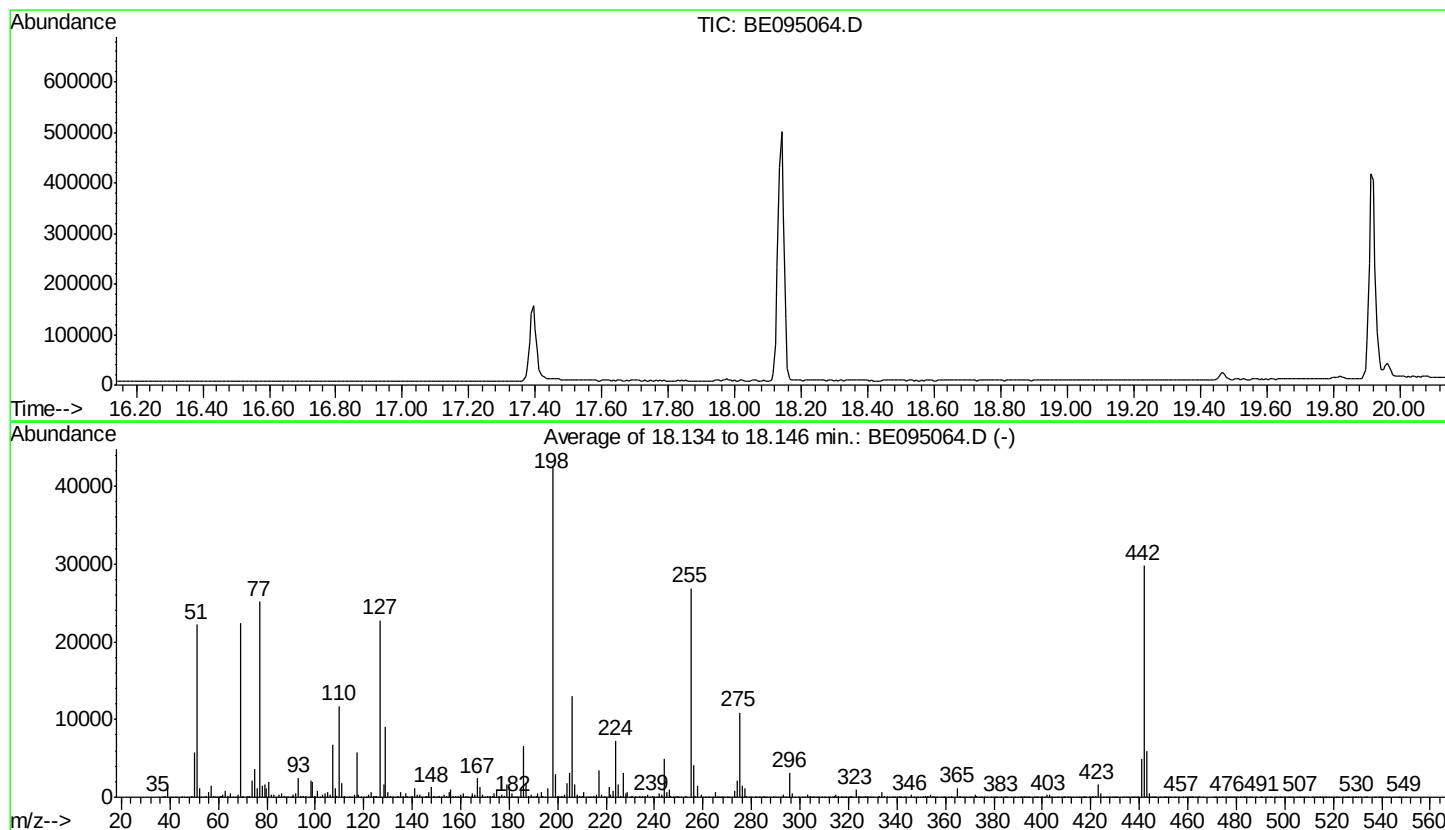

AutoFind: Scans 2646, 2647, 2648; Background Corrected with Scan 2639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.0	22171	PASS
68	69	0.00	2	1.2	275	PASS
69	198	0.00	100	52.4	22359	PASS
70	69	0.00	2	0.4	90	PASS
127	198	10	80	53.3	22735	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	42675	PASS
199	198	5	9	6.9	2929	PASS
275	198	10	60	25.5	10899	PASS
365	198	1	100	2.9	1235	PASS
441	442	0.01	24	16.7	4961	PASS
442	198	50	100	69.8	29769	PASS
443	442	15	24	19.8	5898	PASS