


Data Path : Z:\HPCHEM1\BNA E\DATA\BE011117\
 Data File : BE092636.D
 Acq On : 11 Jan 2017 11:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 19 16:16:32 2016

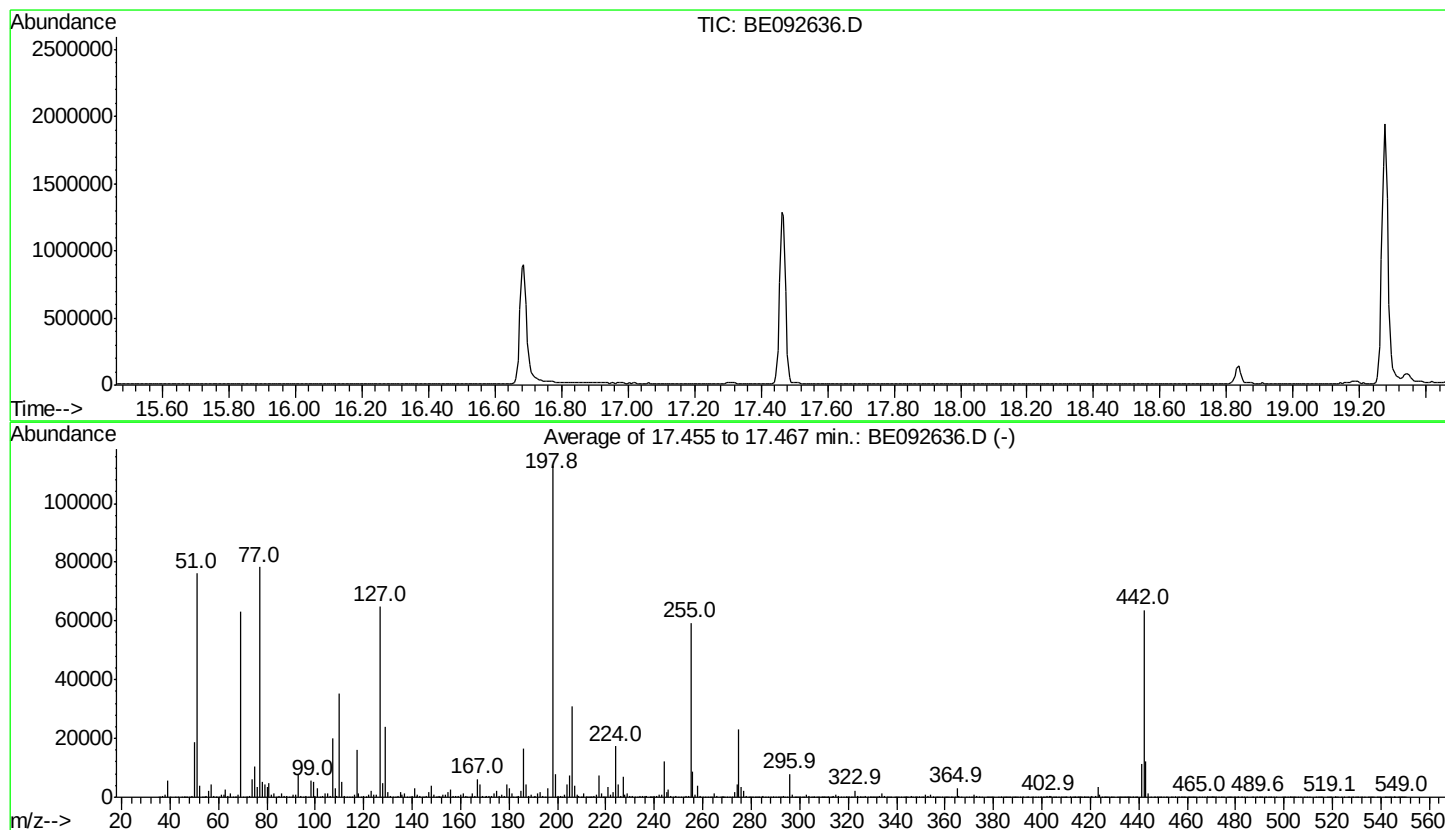

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.5	76153	PASS
68	69	0.00	2	1.6	1015	PASS
69	198	0.00	100	55.8	62972	PASS
70	69	0.00	2	0.4	230	PASS
127	198	10	80	57.5	64866	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	112865	PASS
199	198	5	9	6.9	7745	PASS
275	198	10	60	20.4	23050	PASS
365	198	1	100	2.8	3164	PASS
441	442	0.01	24	17.5	11131	PASS
442	198	50	100	56.4	63712	PASS
443	442	15	24	18.9	12025	PASS