


Data Path : Z:\HPCHEM1\BNA_E\Data\BE011416\
Data File : BE091353.D
Acq On : 14 Jan 2016 16:11
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011416.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 15 15:14:26 2016

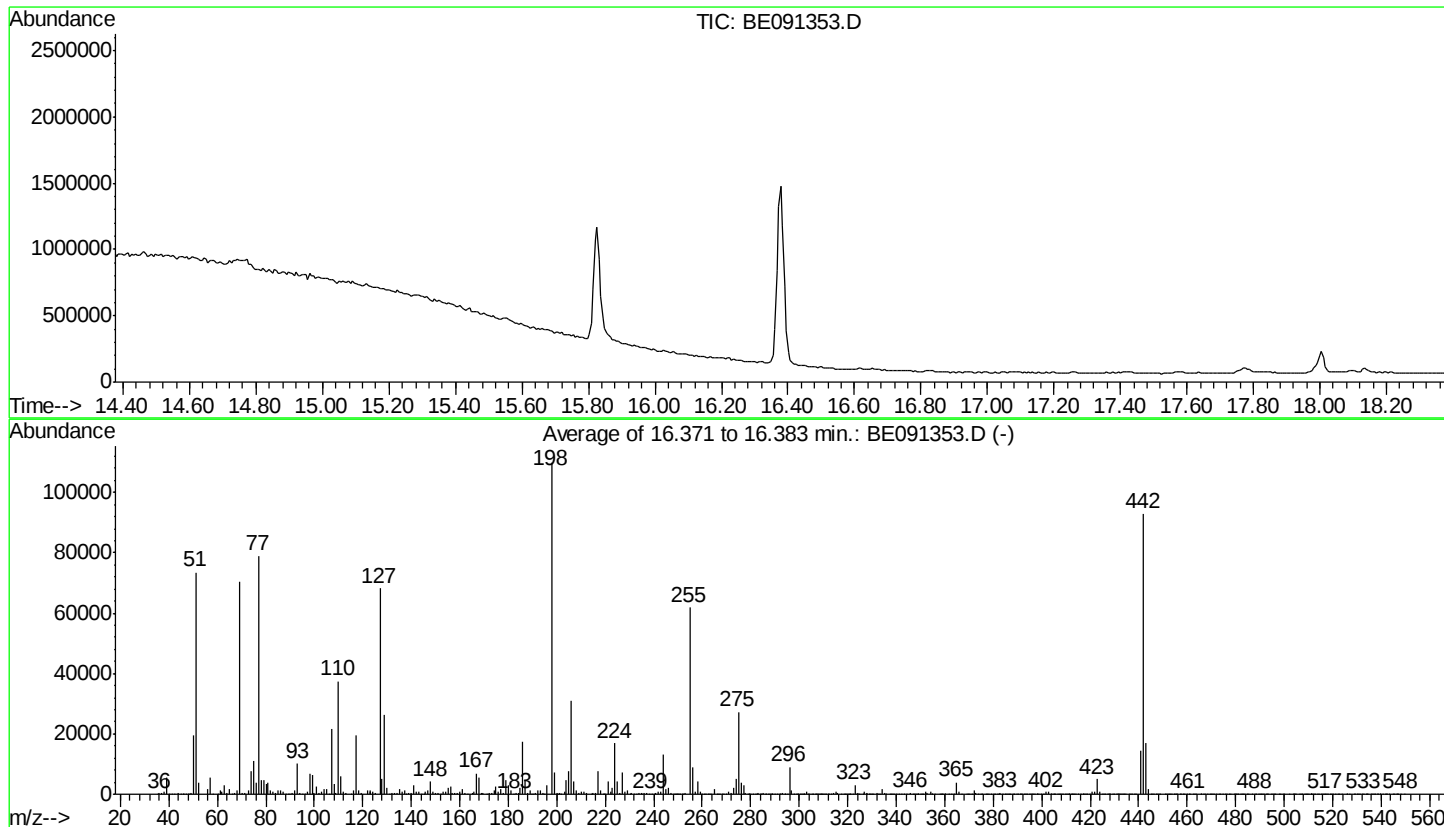

AutoFind: Scans 2346, 2347, 2348; Background Corrected with Scan 2336

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.9	73485	PASS
68	69	0.00	2	1.7	1210	PASS
69	198	0.00	100	64.1	70422	PASS
70	69	0.00	2	0.7	509	PASS
127	198	10	80	62.0	68112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	109859	PASS
199	198	5	9	6.4	7085	PASS
275	198	10	60	24.8	27259	PASS
365	198	1	100	3.5	3830	PASS
441	442	0.01	24	15.7	14627	PASS
442	198	50	100	84.6	92904	PASS
443	442	15	24	18.4	17107	PASS