


Data Path : Z:\HPCHEM1\BNA E\DATA\BE011516\
Data File : BE091371.D
Acq On : 15 Jan 2016 9:00
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011416.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 15 15:14:26 2016

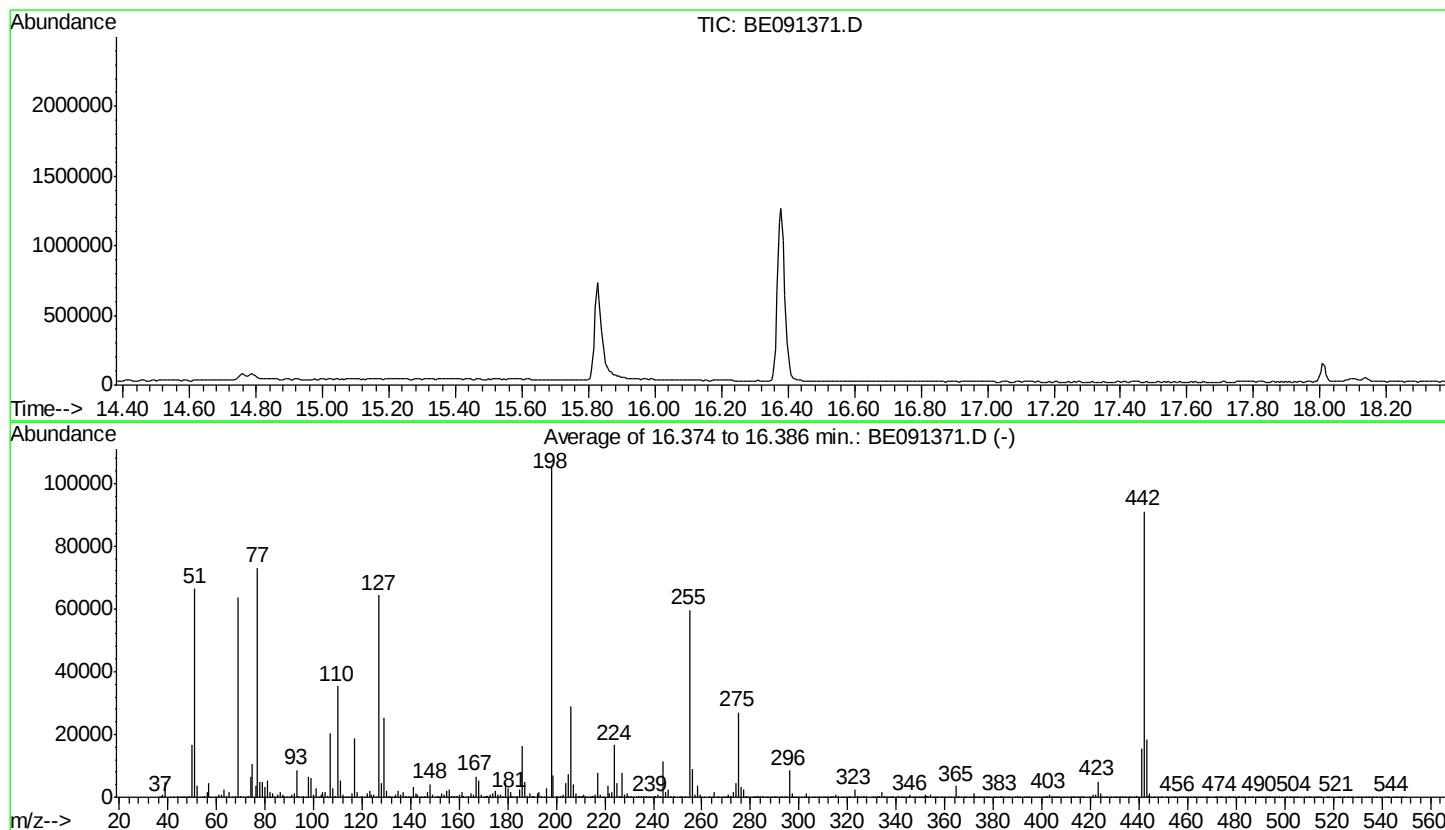

AutoFind: Scans 2346, 2347, 2348; Background Corrected with Scan 2337

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.8	66353	PASS
68	69	0.00	2	0.5	336	PASS
69	198	0.00	100	60.1	63451	PASS
70	69	0.00	2	0.5	323	PASS
127	198	10	80	60.9	64330	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	105616	PASS
199	198	5	9	6.7	7081	PASS
275	198	10	60	25.5	26929	PASS
365	198	1	100	3.4	3589	PASS
441	442	0.01	24	17.1	15564	PASS
442	198	50	100	86.2	91090	PASS
443	442	15	24	20.0	18248	PASS