


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE011520\
 Data File : BE101059.D
 Acq On : 15 Jan 2020 15:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 18:36:25 2020

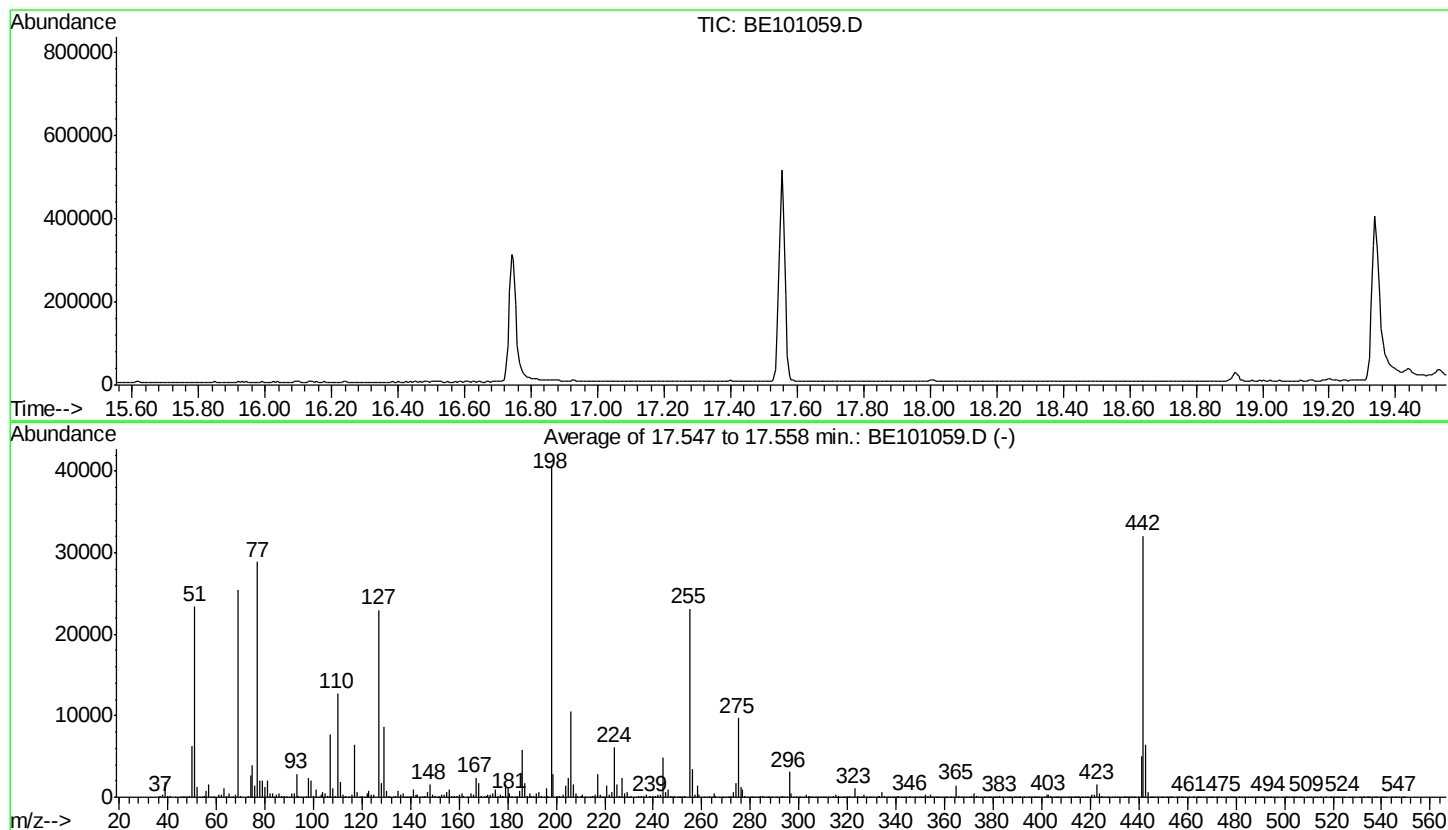

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.4	23345	PASS
68	69	0.00	2	1.5	372	PASS
69	198	0.00	100	62.5	25439	PASS
70	69	0.00	2	0.6	140	PASS
127	198	10	80	56.4	22950	PASS
197	198	0.00	2	0.5	206	PASS
198	198	100	100	100.0	40695	PASS
199	198	5	9	6.9	2790	PASS
275	198	10	60	23.9	9726	PASS
365	198	1	100	3.5	1444	PASS
441	198	0.01	100	12.2	4974	PASS
442	198	50	100	78.9	32096	PASS
443	442	15	24	20.0	6424	PASS