


Data Path : Z:\HPCHEM1\BNA E\DATA\BE011617\
 Data File : BE092647.D
 Acq On : 16 Jan 2017 11:59
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 17 10:14:01 2017

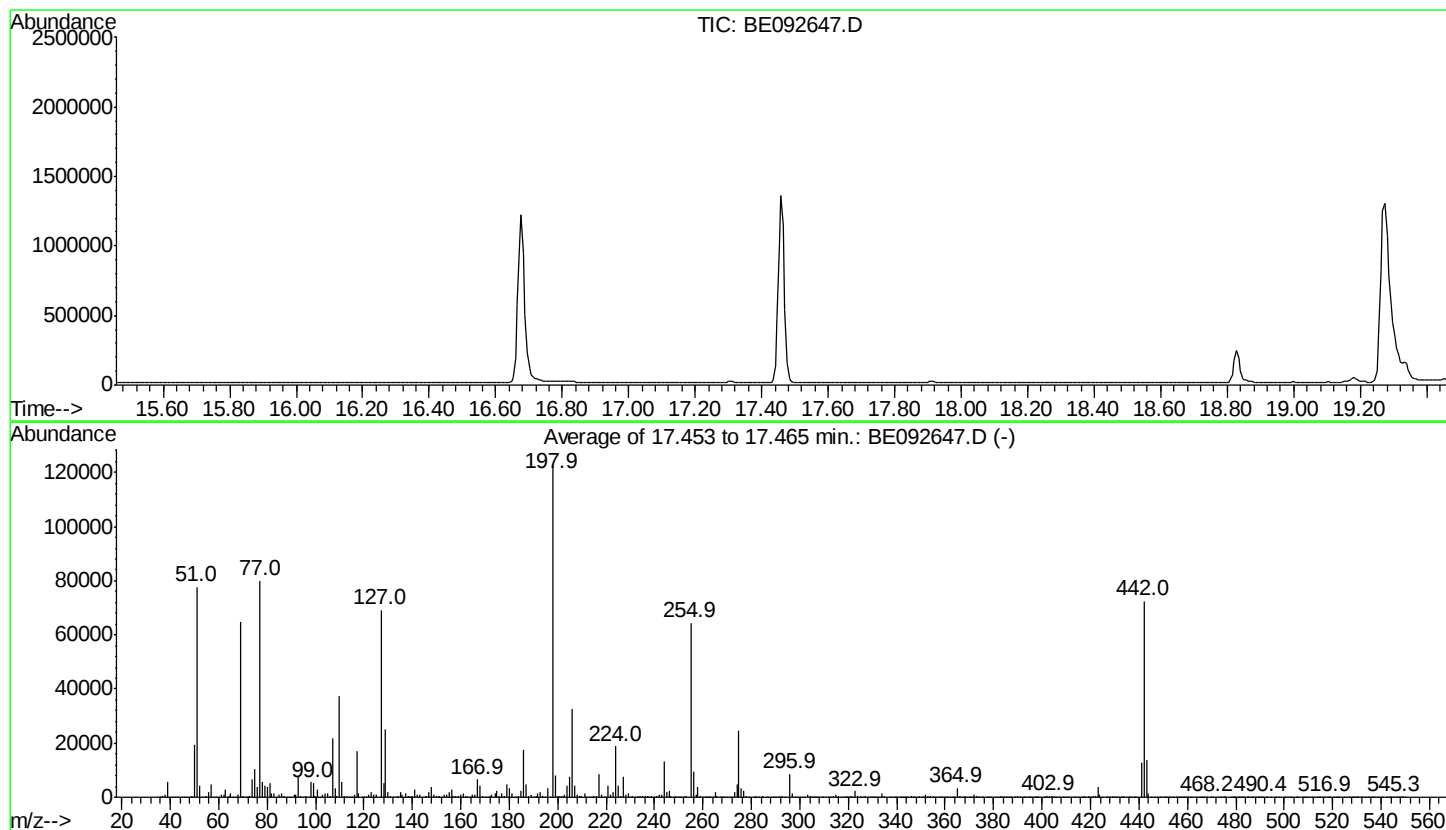

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.4	77717	PASS
68	69	0.00	2	1.6	1031	PASS
69	198	0.00	100	52.7	64609	PASS
70	69	0.00	2	0.5	296	PASS
127	198	10	80	56.5	69234	PASS
197	198	0.00	2	0.1	148	PASS
198	198	100	100	100.0	122530	PASS
199	198	5	9	6.7	8232	PASS
275	198	10	60	20.2	24726	PASS
365	198	1	100	2.8	3488	PASS
441	442	0.01	24	17.4	12645	PASS
442	198	50	100	59.2	72485	PASS
443	442	15	24	18.9	13723	PASS