

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011620\
 Data File : BE101070.D
 Acq On : 16 Jan 2020 10:37
 Operator : JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Manual Integrations
 APPROVED

mohammad
 1/17/2020 2:10:27 PM

Quant Time: Jan 17 13:03:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE010820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 08 18:36:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	2668	0.40	ng	0.00
7) Naphthalene-d8	10.50	136	11878	0.40	ng	0.00
13) Acenaphthene-d10	14.36	164	6763	0.40	ng	0.00
19) Phenanthrene-d10	17.09	188	14795	0.40	ng	0.00
27) Chrysene-d12	21.27	240	14422	0.40	ng	-0.01
34) Perylene-d12	23.69	264	19375	0.40	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.33	112	2612	0.43	ng	0.00
5) Phenol-d6	6.91	99	3079	0.41	ng	0.00
8) Nitrobenzene-d5	8.87	82	3131	0.37	ng	0.00
11) 2-Methylnaphthalene-d10	12.11	152	8914	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.85	330	708	0.37	ng	0.00
15) 2-Fluorobiphenyl	12.99	172	10591	0.41	ng	-0.01
25) Fluoranthene-d10	19.13	212	80216	0.39	ng	0.00
29) Terphenyl-d14	19.73	244	12669	0.36	ng	0.00

Target Compounds					Qvalue
2) 1,4-Dioxane	3.28	88	2785	0.447 ng	98
3) n-Nitrosodimethylamine	3.60	42	1446	0.390 ng	95
6) bis(2-Chloroethyl)ether	7.16	93	3234	0.357 ng	94
9) Naphthalene	10.55	128	54224	0.411 ng	100
10) Hexachlorobutadiene	10.83	225	2435	0.436 ng	98
12) 2-Methylnaphthalene	12.18	142	7357	0.369 ng	98
16) Acenaphthylene	14.07	152	11357	0.412 ng	99
17) Acenaphthene	14.41	154	8050	0.408 ng	97
18) Fluorene	15.39	166	9491	0.381 ng	100
20) 4-Bromophenyl-phenylether	16.30	248	2700	0.374 ng	93
21) Hexachlorobenzene	16.40	284	3278	0.414 ng	98
22) Pentachlorophenol	16.76	266	552	0.449 ng	100
23) Phenanthrene	17.13	178	15612	0.386 ng	100
24) Anthracene	17.23	178	15171	0.398 ng	99
26) Fluoranthene	19.16	202	19694	0.389 ng	99
28) Pyrene	19.51	202	20286	0.378 ng	99
30) Benzo(a)anthracene	21.26	228	15633	0.380 ng	99
31) Chrysene	21.31	228	25784	0.422 ng	98
32) Bis(2-ethylhexyl)phthalate	21.20	149	29237	0.426 ng	99
33) Indeno(1,2,3-cd)pyrene	26.24	276	24583	0.509 ng	# 94
35) Benzo(b)fluoranthene	22.95	252	18094	0.333 ng	99
36) Benzo(k)fluoranthene	23.00	252	29072m	0.369 ng	
37) Benzo(a)pyrene	23.58	252	20343	0.387 ng	98
38) Dibenzo(a,h)anthracene	26.26	278	19064	0.394 ng	94
39) Benzo(g,h,i)perylene	27.01	276	22579	0.380 ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011620\
Data File : BE101070.D
Acq On : 16 Jan 2020 10:37
Operator : JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM

Quant Time: Jan 17 13:03:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 18:36:25 2020
Response via : Initial Calibration

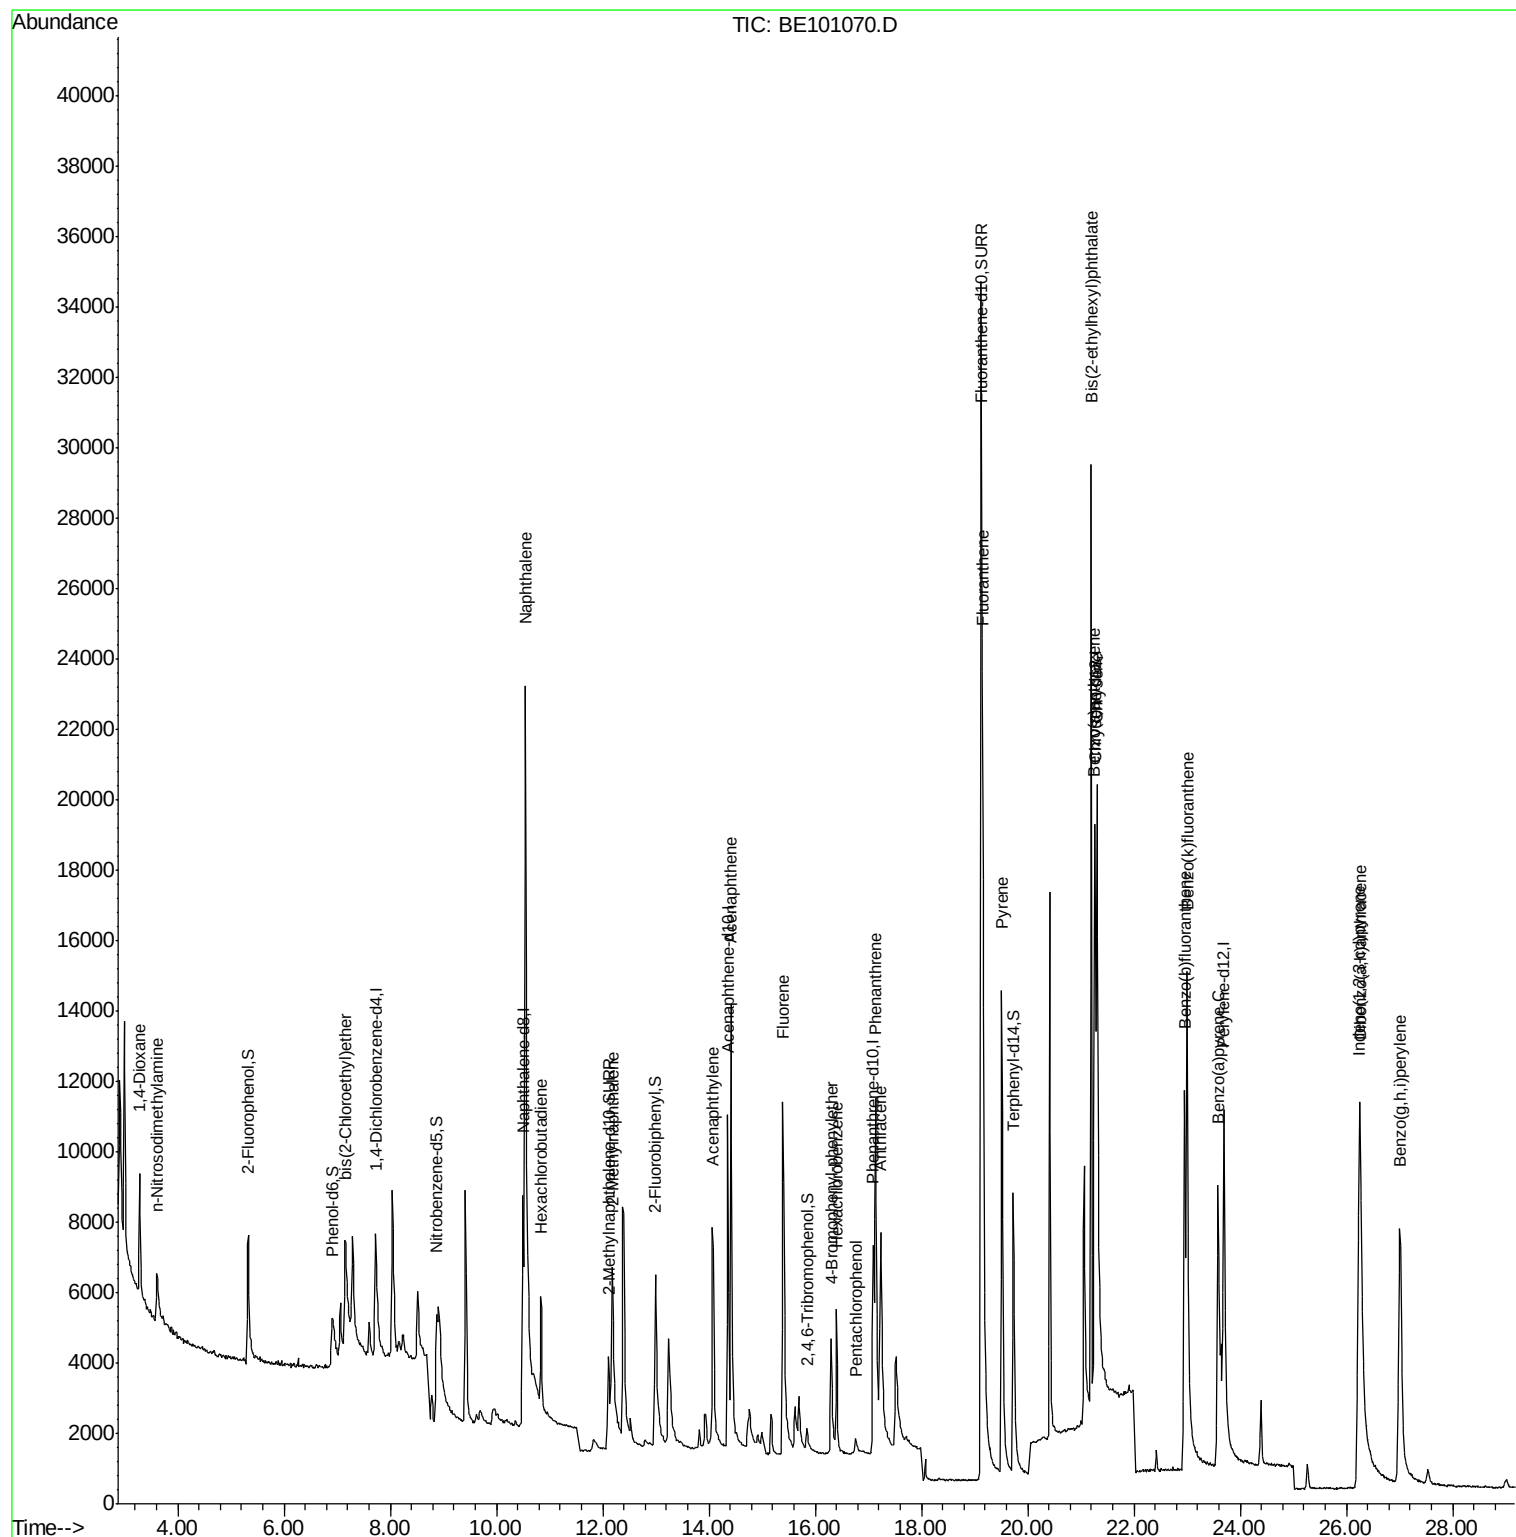



#1





1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.73 min Scan# 422
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.5	120.3	180.5
115	70.0	51.7	77.5

Manual Integrations
APPROVED




mohammad
1/17/2020 2:10:27 PM






#2

1,4-Dioxane
Concen: 0.447 ng
RT: 3.28 min Scan# 36
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
88	100		
58	68.1	53.0	79.4
43	28.3	23.4	35.2



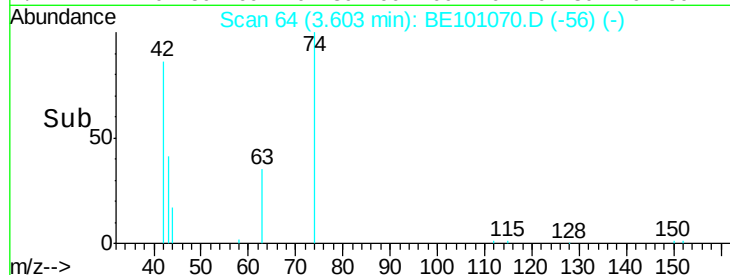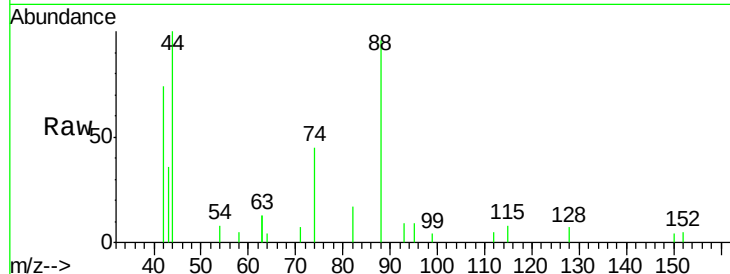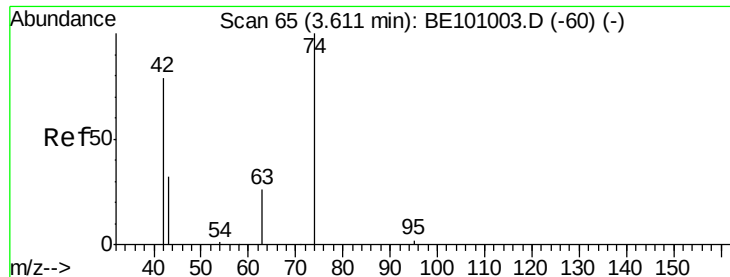





#3
n-Nitrosodimethylamine
Concen: 0.390 ng
RT: 3.60 min Scan# 64
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tot Ion: 42 Resp: 1446
Ion Ratio Lower Upper
42 100
74 125.8 105.7 158.5
44 11.4 10.0 15.0

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4


Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:27 PM

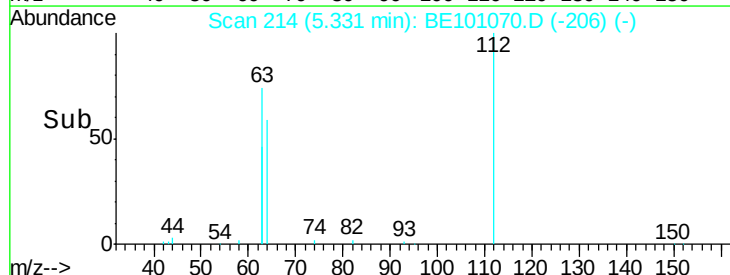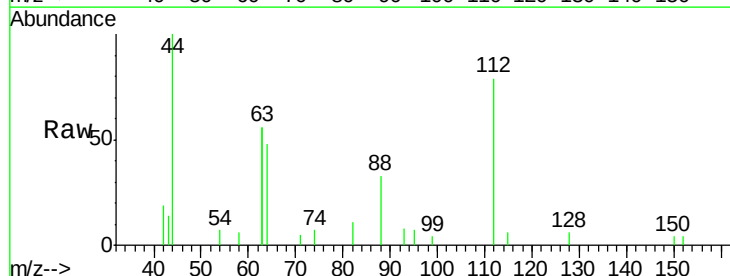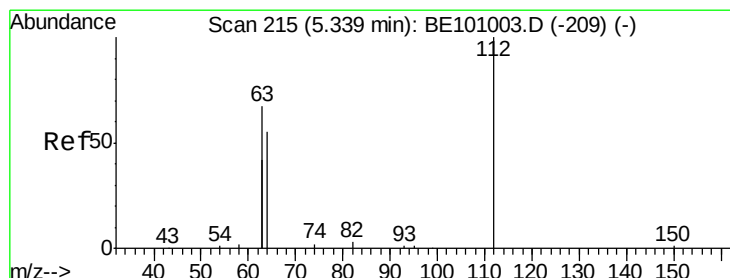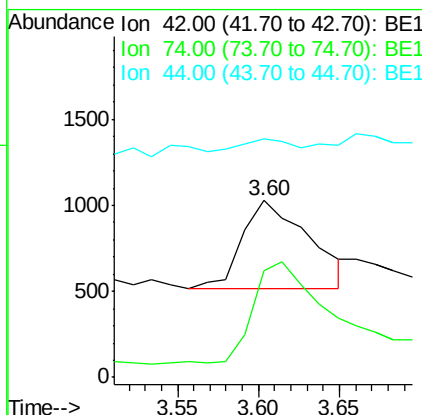

#4
2-Fluorophenol
Concen: 0.435 ng
RT: 5.33 min Scan# 214
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion: 112 Resp: 2612
Ion Ratio Lower Upper
112 100
64 69.0 53.6 80.4
63 151.2 114.6 172.0

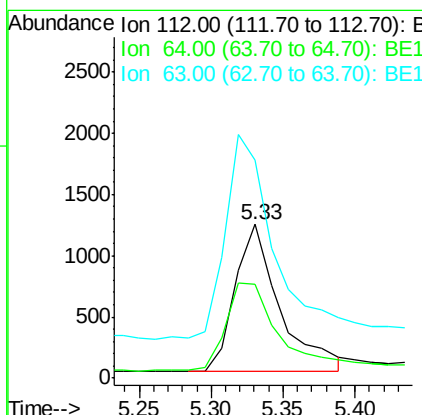

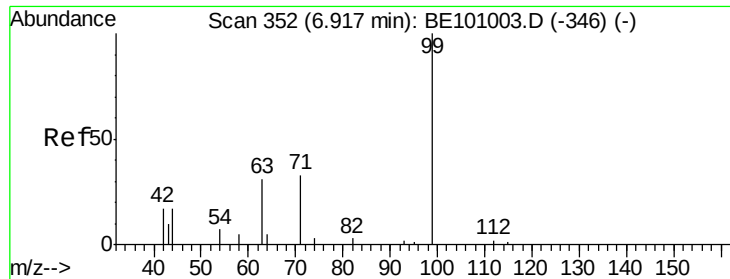

#5

Phenol-d6

Concen: 0.405 ng

RT: 6.91 min Scan# 351

Delta R.T. -0.01 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion:	99	Resp:	3079
Ion	Ratio	Lower	Upper
99	100		
42	23.1	18.3	27.5
71	38.1	28.0	42.0

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM

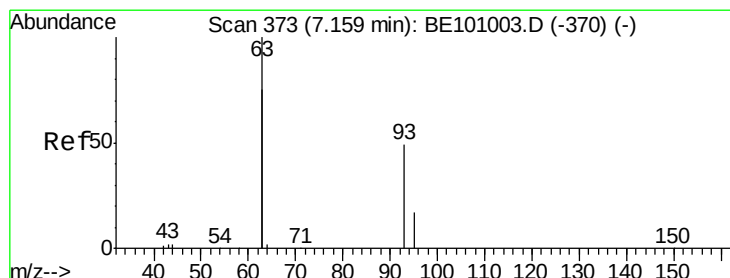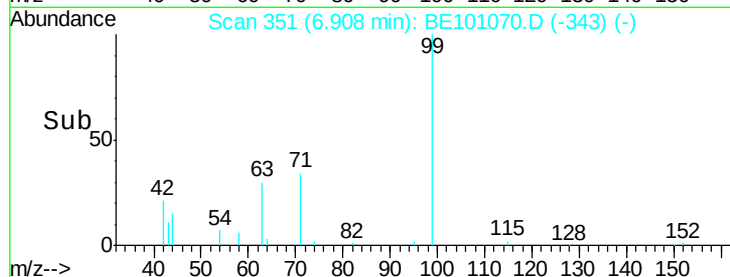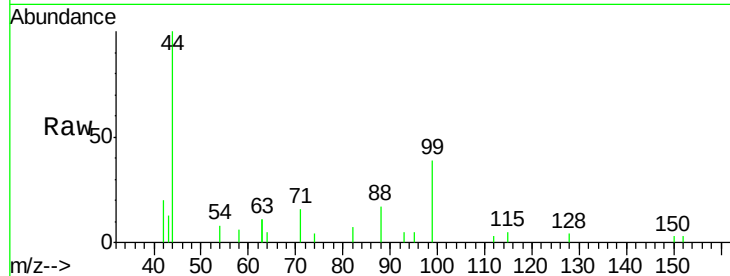

#6

bis(2-Chloroethyl)ether

Concen: 0.357 ng




RT: 7.16 min Scan# 373


Delta R.T. 0.00 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Tgt Ion:	93	Resp:	3234
Ion	Ratio	Lower	Upper
93	100		
63	281.0	233.9	350.9
95	31.6	23.5	35.3

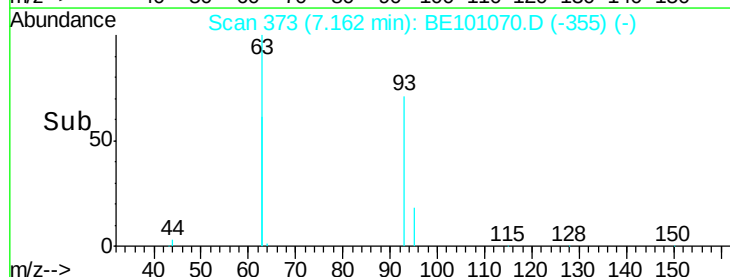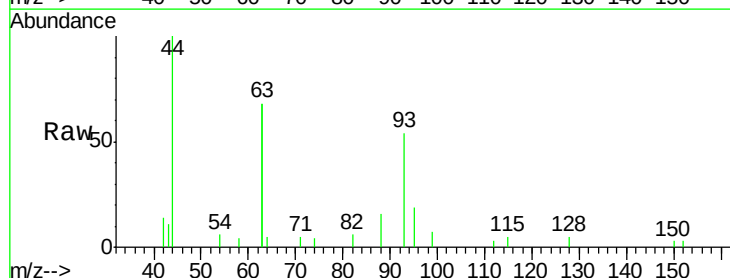



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.50 min Scan# 641

Delta R.T. -0.00 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Instrument :

BNA_E


ClientSampleId :

SSTDCCC0.4




Tot Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.3	13.9
54	38.7	36.8	55.2
68	8.3	8.4	12.6

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BE1
Ion 68.00 (67.70 to 68.70): BE1

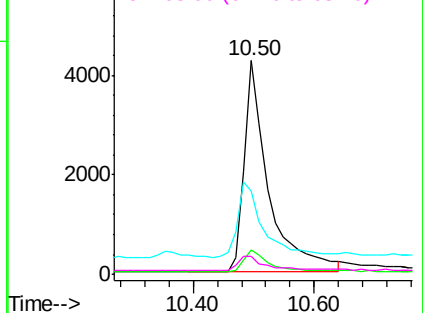

#8

Nitrobenzene-d5

Concen: 0.369 ng


RT: 8.87 min Scan# 516

Delta R.T. -0.00 min



Lab File: BE101070.D


Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
82	100		
128	147.8	109.8	164.6
54	233.6	174.5	261.7



Abundance Ion 82.00 (81.70 to 82.70): BE1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BE1

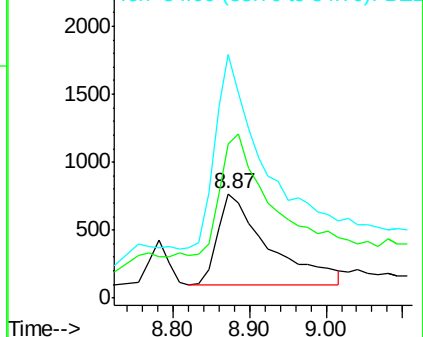

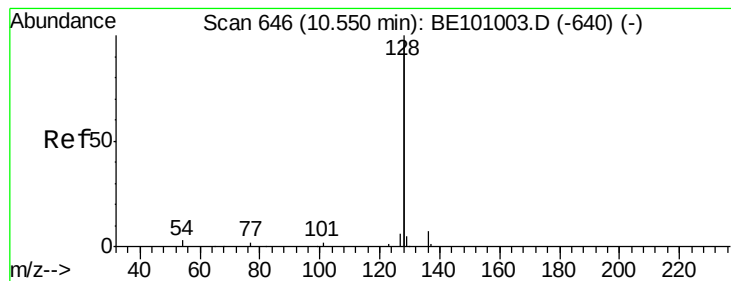

#9

Naphthalene

Concen: 0.411 ng

RT: 10.55 min Scan# 645

Delta R.T. -0.00 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion:	128	Resp:	54224
Ion	Ratio	Lower	Upper
128	100		
129	3.1	2.3	3.5
127	3.5	2.7	4.1

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM

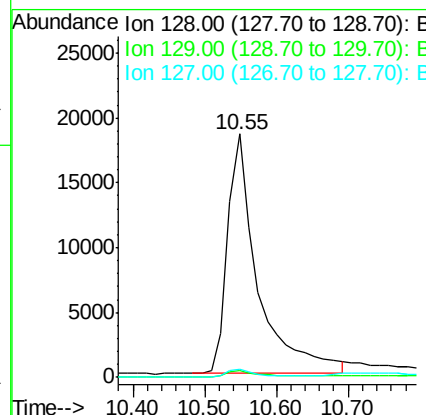

#10

Hexachlorobutadiene

Concen: 0.436 ng




RT: 10.83 min Scan# 667


Delta R.T. -0.01 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Tgt Ion:	225	Resp:	2435
Ion	Ratio	Lower	Upper
225	100		
223	61.9	52.2	78.4
227	62.3	49.9	74.9



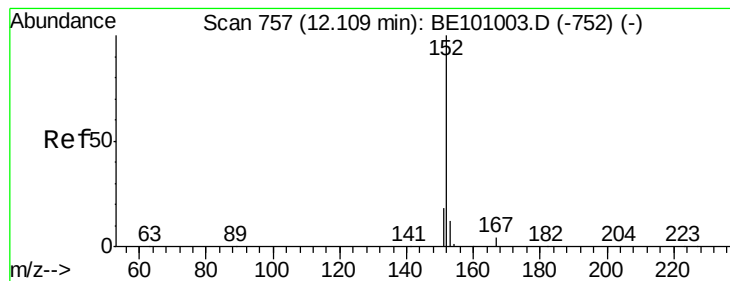





#11
 2-Methylnaphthalene-d10
 Concen: 0.393 ng
 RT: 12.11 min Scan# 756
 Delta R.T. 0.00 min
 Lab File: BE101070.D
 Acq: 16 Jan 2020 10:37

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
152	100		
151	19.1	15.0	22.6




Manual Integrations
 APPROVED


mohammad
 1/17/2020 2:10:27 PM

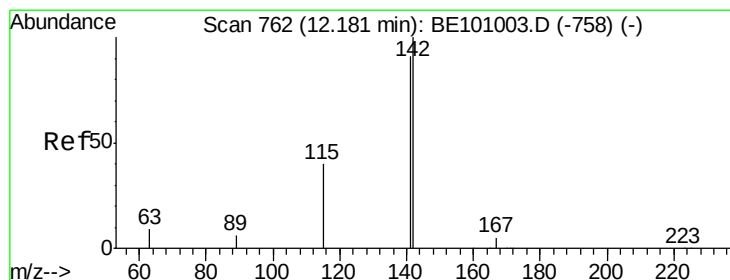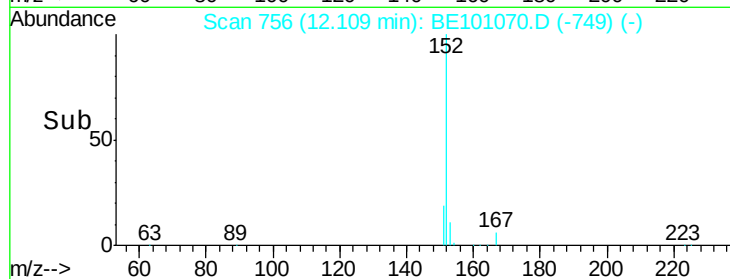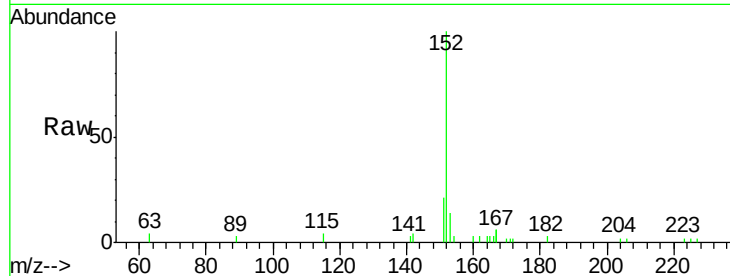

#12
 2-Methylnaphthalene
 Concen: 0.369 ng
 RT: 12.18 min Scan# 761
 Delta R.T. 0.00 min
 Lab File: BE101070.D
 Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
142	100		
141	87.5	72.5	108.7
115	41.6	33.0	49.6

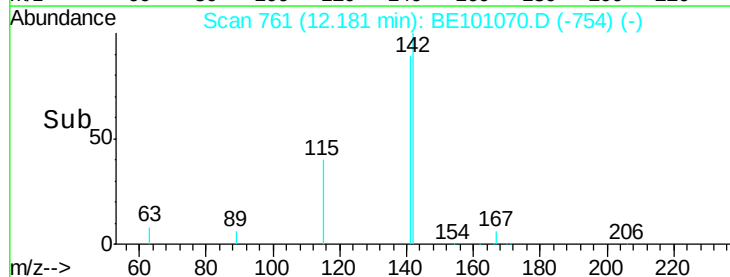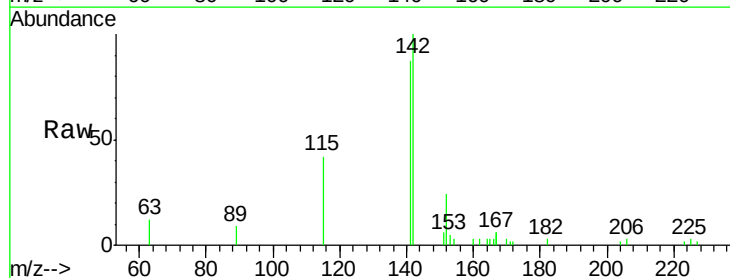







#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.36 min Scan# 912
Delta R.T. 0.00 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
164	100		
162	103.6	84.1	126.1
160	50.1	40.4	60.6




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:27 PM

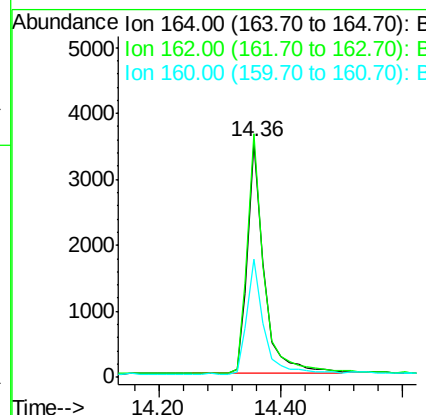

#14
2,4,6-Tribromophenol
Concen: 0.371 ng
RT: 15.85 min Scan# 1017
Delta R.T. 0.00 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
330	100		
332	91.2	78.4	117.6
141	41.8	37.0	55.4

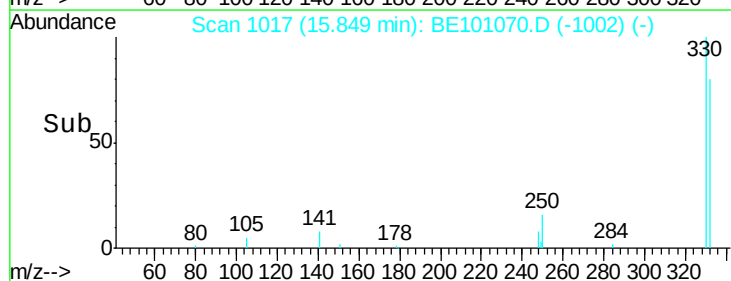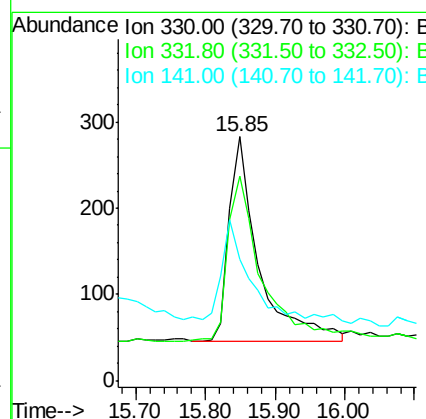







#15
2-Fluorobiphenyl
Concen: 0.412 ng
RT: 12.99 min Scan# 817
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
172	100		
171	36.5	28.2	42.2
170	24.5	18.9	28.3




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:27 PM



#16
Acenaphthylene
Concen: 0.412 ng
RT: 14.07 min Scan# 892
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
152	100		
151	20.2	15.5	23.3
153	13.2	10.4	15.6






#17
Acenaphthene
Concen: 0.408 ng
RT: 14.41 min Scan# 916
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
154	100		
153	112.7	93.6	140.4
152	57.3	46.3	69.5

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM






Abundance

Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

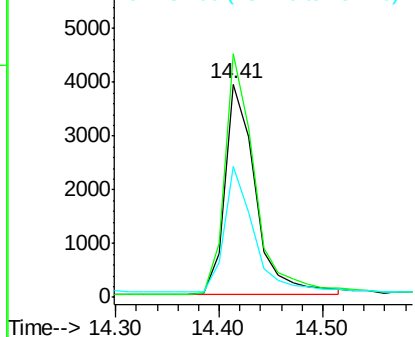

#18
Fluorene
Concen: 0.381 ng
RT: 15.39 min Scan# 983
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37




Tgt Ion	Ratio	Lower	Upper
166	100		
165	100.0	79.8	119.8
167	13.6	11.0	16.6


Abundance

Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

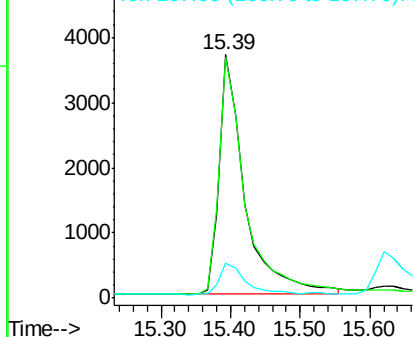







#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.09 min Scan# 1110
Delta R.T. 0.00 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	12.3	10.8	16.2




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:27 PM

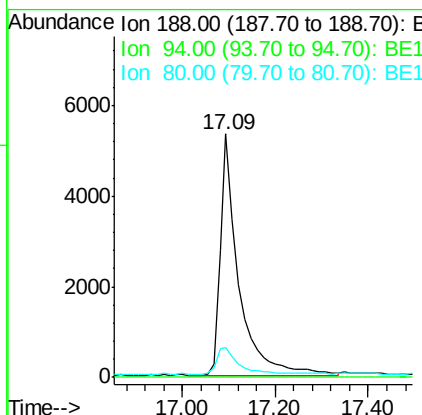

#20
4-Bromophenyl-phenylether
Concen: 0.374 ng
RT: 16.30 min Scan# 1051
Delta R.T. 0.00 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
248	100		
250	106.1	76.6	115.0
141	69.8	57.7	86.5

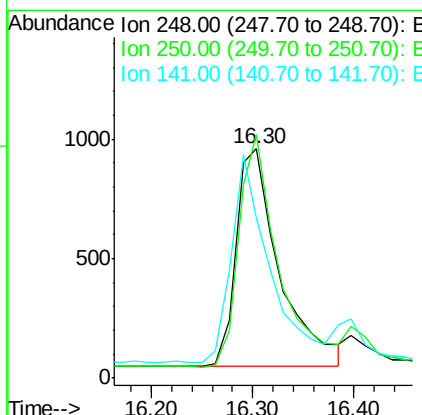







#21
Hexachlorobenzene
Concen: 0.414 ng
RT: 16.40 min Scan# 1058
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
284	100		
142	42.8	34.0	51.0
249	33.7	28.2	42.4




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:27 PM

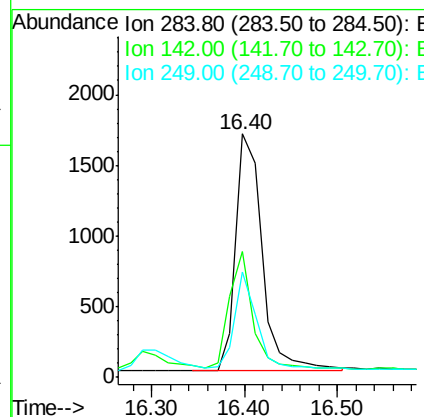

#22
Pentachlorophenol
Concen: 0.449 ng
RT: 16.76 min Scan# 1085
Delta R.T. 0.00 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
266	100		
264	75.9	61.0	91.4
268	72.7	58.5	87.7

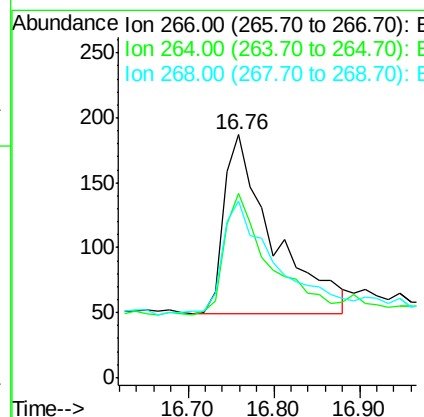



#23

Phenanthrene

Concen: 0.386 ng

RT: 17.13 min Scan# 1113

Delta R.T. 0.00 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion:	178	Resp:	15612
Ion Ratio	Lower	Upper	
178	100		
176	19.4	15.7	23.5
179	15.1	12.0	18.0

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM

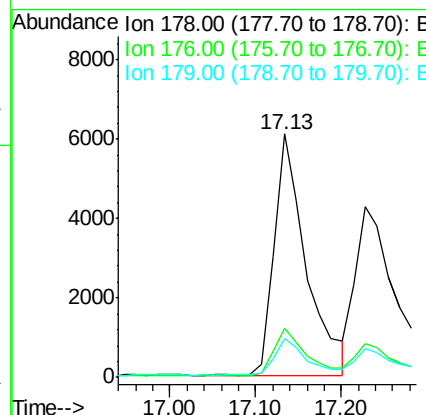

#24

Anthracene

Concen: 0.398 ng




RT: 17.23 min Scan# 1120


Delta R.T. 0.00 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Tgt Ion:	178	Resp:	15171
Ion Ratio	Lower	Upper	
178	100		
176	18.0	14.8	22.2
179	15.1	12.4	18.6





#25

Fluoranthene-d10

Concen: 0.390 ng

RT: 19.13 min Scan# 1368

Delta R.T. -0.01 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion:	212	Resp:	80216
Ion Ratio	Lower	Upper	
212	100		
106	3.4	2.6	3.8
104	1.8	1.4	2.0

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM



#26

Fluoranthene

Concen: 0.389 ng




RT: 19.16 min Scan# 1373


Delta R.T. -0.01 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Tgt Ion:	202	Resp:	19694
Ion Ratio	Lower	Upper	
202	100		
101	11.7	9.6	14.4
203	16.7	13.8	20.6





#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.27 min Scan# 1622

Delta R.T. -0.01 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Instrument :

BNA_E





ClientSampleId :

SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
240	100		
120	14.0	8.6	13.0#
236	28.2	22.2	33.4

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM

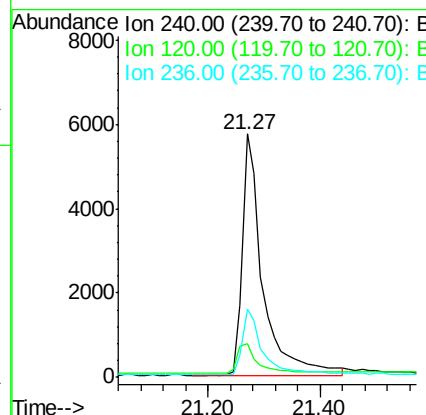

#28

Pyrene

Concen: 0.378 ng




RT: 19.51 min Scan# 1435


Delta R.T. -0.01 min

Lab File: BE101070.D

Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
202	100		
200	20.8	17.0	25.4
203	17.2	13.8	20.6









#29
 Terphenyl-d14
 Concen: 0.358 ng
 RT: 19.73 min Scan# 1473
 Delta R.T. -0.01 min
 Lab File: BE101070.D
 Acq: 16 Jan 2020 10:37

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
244	100		
212	35.7	27.2	40.8
122	14.0	9.8	14.8




Manual Integrations
 APPROVED


mohammad
 1/17/2020 2:10:27 PM



#30
 Benzo(a)anthracene
 Concen: 0.380 ng
 RT: 21.26 min Scan# 1621
 Delta R.T. -0.00 min
 Lab File: BE101070.D
 Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.8	22.7	34.1
229	20.2	15.5	23.3






#31
Chrysene
Concen: 0.422 ng
RT: 21.31 min Scan# 1625
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4




Tot Ion:228	Resp:	25784
Ion Ratio	Lower	Upper
228 100		
226 29.9	23.5	35.3
229 19.1	16.7	25.1

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:27 PM






Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

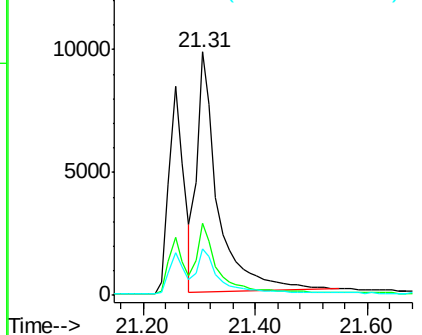


#32
Bis(2-ethylhexyl)phthalate
Concen: 0.426 ng
RT: 21.20 min Scan# 1616
Delta R.T. -0.00 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion:149	Resp:	29237
Ion Ratio	Lower	Upper
149 100		
167 6.7	5.2	7.8
279 0.9	0.8	1.2

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

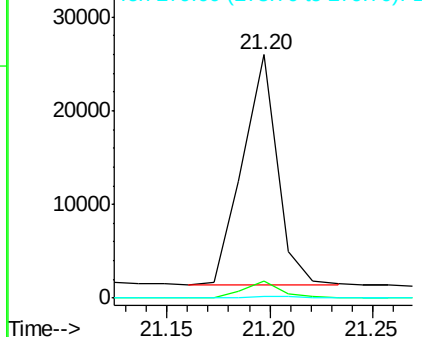







#33
Indeno(1,2,3-cd)pyrene
Concen: 0.509 ng
RT: 26.24 min Scan# 2860
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
276	100		
138	25.3	16.1	24.1#
277	21.9	18.1	27.1




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:27 PM



#34
Perylene-d12
Concen: 0.400 ng
RT: 23.69 min Scan# 2151
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.7	20.3	30.5
265	27.8	27.0	40.4



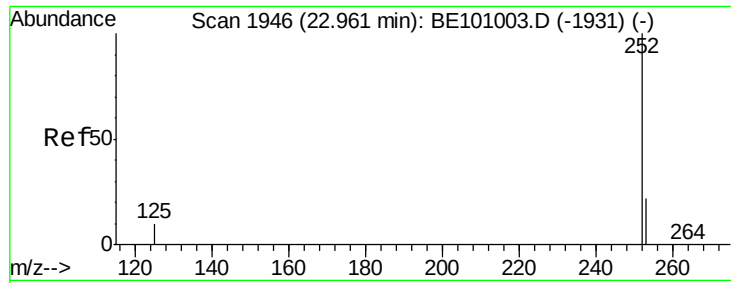





#35
Benzo(b)fluoranthene
Concen: 0.333 ng
RT: 22.95 min Scan# 1943
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.4	18.5	27.7
125	11.8	9.5	14.3




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:27 PM



#36
Benzo(k)fluoranthene
Concen: 0.369 ng m
RT: 23.00 min Scan# 1956
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.7	18.9	28.3
125	19.2	10.1	15.1#



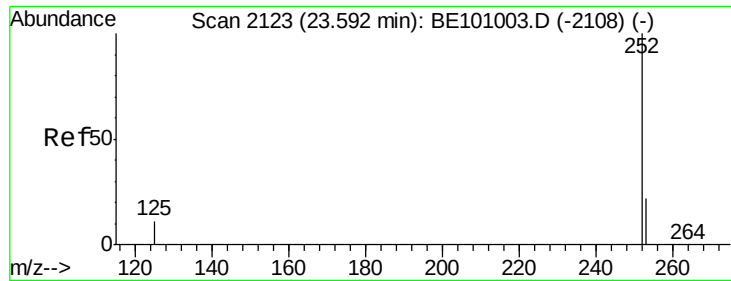





#37
Benzo(a)pyrene
Concen: 0.387 ng
RT: 23.58 min Scan# 2120
Delta R.T. -0.01 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Instrument :
BNA_E
ClientSampleId :
SSTDCCC0.4

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.3	19.4	29.2
125	13.9	11.8	17.6




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:27 PM



#38
Dibenzo(a,h)anthracene
Concen: 0.394 ng
RT: 26.26 min Scan# 2865
Delta R.T. -0.02 min
Lab File: BE101070.D
Acq: 16 Jan 2020 10:37

Tgt Ion	Ratio	Lower	Upper
278	100		
139	19.0	15.0	22.4
279	23.5	22.6	33.8





#39
 Benzo(a,h,i)perylene
 Concen: 0.380 ng
 RT: 27.01 min Scan# 3077
 Delta R.T. -0.01 min
 Lab File: BE101070.D
 Acq: 16 Jan 2020 10:37

Instrument :
 BNA_E
 ClientSampleId :
 SSTDCCC0.4

Tot Ion:	276	Resp:	22579
Ion Ratio	Lower	Upper	
276	100		
277	23.7	19.4	29.2
138	22.7	17.9	26.9

Manual Integrations
 APPROVED

mohammad
 1/17/2020 2:10:27 PM

