

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011620\
 Data File : BE101076.D
 Acq On : 16 Jan 2020 15:23
 Operator : JU
 Sample : PB126135BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 PB126135BS

Manual Integrations
 APPROVED

mohammad
 1/17/2020 2:10:34 PM

Quant Time: Jan 17 13:05:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE010820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 08 18:36:25 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	2970	0.40	ng	-0.01
7) Naphthalene-d8	10.50	136	12636	0.40	ng	0.00
13) Acenaphthene-d10	14.36	164	7697	0.40	ng	0.00
19) Phenanthrene-d10	17.09	188	16559	0.40	ng	0.00
27) Chrysene-d12	21.27	240	16243	0.40	ng	-0.01
34) Perylene-d12	23.69	264	21195	0.40	ng	0.00

System Monitoring Compounds						
4) 2-Fluorophenol	5.33	112	3072	0.46	ng	-0.01
5) Phenol-d6	6.90	99	3562	0.42	ng	-0.01
8) Nitrobenzene-d5	8.87	82	3671	0.41	ng	0.00
11) 2-Methylnaphthalene-d10	12.09	152	8743	0.36	ng	-0.02
14) 2,4,6-Tribromophenol	15.84	330	799	0.37	ng	-0.01
15) 2-Fluorobiphenyl	12.99	172	11170	0.38	ng	-0.02
25) Fluoranthene-d10	19.12	212	91776	0.40	ng	-0.01
29) Terphenyl-d14	19.73	244	15189	0.38	ng	0.00

Target Compounds				Qvalue		
2) 1,4-Dioxane	3.29	88	3130	0.453	ng	97
3) n-Nitrosodimethylamine	3.60	42	1660	0.402	ng	# 93
6) bis(2-Chloroethyl)ether	7.16	93	3737	0.371	ng	95
9) Naphthalene	10.55	128	57671	0.411	ng	100
10) Hexachlorobutadiene	10.84	225	2629	0.442	ng	96
12) 2-Methylnaphthalene	12.17	142	8044	0.379	ng	99
16) Acenaphthylene	14.07	152	12745	0.407	ng	99
17) Acenaphthene	14.41	154	8771	0.391	ng	97
18) Fluorene	15.39	166	10579	0.373	ng	98
20) 4-Bromophenyl-phenylether	16.29	248	3014	0.373	ng	98
21) Hexachlorobenzene	16.40	284	3565	0.402	ng	99
22) Pentachlorophenol	16.75	266	785	0.503	ng	91
23) Phenanthrene	17.13	178	17403	0.385	ng	99
24) Anthracene	17.23	178	17658	0.414	ng	100
26) Fluoranthene	19.15	202	22414	0.396	ng	99
28) Pyrene	19.51	202	23610	0.390	ng	100
30) Benzo(a)anthracene	21.26	228	19290	0.416	ng	96
31) Chrysene	21.31	228	28636	0.416	ng	98
32) Bis(2-ethylhexyl)phthalate	21.20	149	42082	0.545	ng	100
33) Indeno(1,2,3-cd)pyrene	26.23	276	26951	0.495	ng	# 93
35) Benzo(b)fluoranthene	22.95	252	20104	0.338	ng	100
36) Benzo(k)fluoranthene	23.00	252	32055m	0.372	ng	
37) Benzo(a)pyrene	23.58	252	22224	0.386	ng	98
38) Dibenzo(a,h)anthracene	26.26	278	21232	0.401	ng	95
39) Benzo(g,h,i)perylene	27.01	276	24167	0.372	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011620\
Data File : BE101076.D
Acq On : 16 Jan 2020 15:23
Operator : JU
Sample : PB126135BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
PB126135BS

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM

Quant Time: Jan 17 13:05:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 18:36:25 2020
Response via : Initial Calibration





#1





1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.72 min Scan# 422
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Instrument :
BNA_E
ClientSampled :
PB126135BS

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.5	120.3	180.5
115	69.2	51.7	77.5

Manual Integrations
APPROVED




mohammad
1/17/2020 2:10:34 PM





#2

1,4-Dioxane
Concen: 0.453 ng
RT: 3.29 min Scan# 37
Delta R.T. 0.00 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
88	100		
58	64.1	53.0	79.4
43	27.0	23.4	35.2





#3

n-Nitrosodimethylamine

Concen: 0.402 ng

RT: 3.60 min Scan# 64

Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tot Ion:	42	Resp:	1660
Ion	Ratio	Lower	Upper
42	100		
74	137.5	105.7	158.5
44	0.0	10.0	15.0#

Instrument :





BNA_E

ClientSampleId :

PB126135BS

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#4

2-Fluorophenol

Concen: 0.460 ng


RT: 5.33 min Scan# 214

Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion:	112	Resp:	3072
Ion	Ratio	Lower	Upper
112	100		
64	72.8	53.6	80.4
63	149.2	114.6	172.0





#5

Phenol-d6

Concen: 0.421 ng

RT: 6.90 min Scan# 351

Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E





ClientSampleId :

PB126135BS

Tot Ion:	99	Resp:	3562
Ion	Ratio	Lower	Upper
99	100		
42	25.3	18.3	27.5
71	35.4	28.0	42.0

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#6

bis(2-Chloroethyl)ether

Concen: 0.371 ng




RT: 7.16 min Scan# 373


Delta R.T. -0.00 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion:	93	Resp:	3737
Ion	Ratio	Lower	Upper
93	100		
63	284.1	233.9	350.9
95	33.5	23.5	35.3





#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.50 min Scan# 641

Delta R.T. -0.00 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E





ClientSampleId :

PB126135BS

Tot Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.3	13.9
54	33.9	36.8	55.2#
68	7.6	8.4	12.6#

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#8

Nitrobenzene-d5

Concen: 0.406 ng




RT: 8.87 min Scan# 516


Delta R.T. -0.00 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
82	100		
128	153.2	109.8	164.6
54	205.1	174.5	261.7





#9

Naphthalene

Concen: 0.411 ng

RT: 10.55 min Scan# 645

Delta R.T. -0.00 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E





ClientSampled :

PB126135BS

Tot Ion:	128	Resp:	57671
Ion	Ratio	Lower	Upper
128	100		
129	3.1	2.3	3.5
127	3.5	2.7	4.1

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#10

Hexachlorobutadiene

Concen: 0.442 ng




RT: 10.84 min Scan# 667

Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion:	225	Resp:	2629
Ion	Ratio	Lower	Upper
225	100		
223	60.4	52.2	78.4
227	61.8	49.9	74.9









#11
2-Methylnaphthalene-d10
Concen: 0.363 ng
RT: 12.09 min Scan# 755
Delta R.T. -0.02 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Instrument :
BNA_E
ClientSampleId :
PB126135BS

Tot Ion	Ratio	Lower	Upper
152	100		
151	20.9	15.0	22.6




Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#12
2-Methylnaphthalene
Concen: 0.379 ng
RT: 12.17 min Scan# 760
Delta R.T. -0.02 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.8	72.5	108.7
115	43.0	33.0	49.6









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.36 min Scan# 912
Delta R.T. -0.00 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Instrument :
BNA_E
ClientSampleId :
PB126135BS

Tot Ion	Ratio	Lower	Upper
164	100		
162	102.8	84.1	126.1
160	47.4	40.4	60.6




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:34 PM



#14
2,4,6-Tribromophenol
Concen: 0.368 ng
RT: 15.84 min Scan# 1016
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
330	100		
332	99.5	78.4	117.6
141	49.3	37.0	55.4






#15
2-Fluorobiphenyl
Concen: 0.382 ng
RT: 12.99 min Scan# 817
Delta R.T. -0.02 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Instrument :
BNA_E
ClientSampleId :
PB126135BS

Tot Ion	Ratio	Lower	Upper
172	100		
171	35.8	28.2	42.2
170	25.1	18.9	28.3

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



#16
Acenaphthylene
Concen: 0.407 ng
RT: 14.07 min Scan# 892
Delta R.T. -0.02 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23




Tgt Ion	Ratio	Lower	Upper
152	100		
151	19.7	15.5	23.3
153	12.9	10.4	15.6


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E



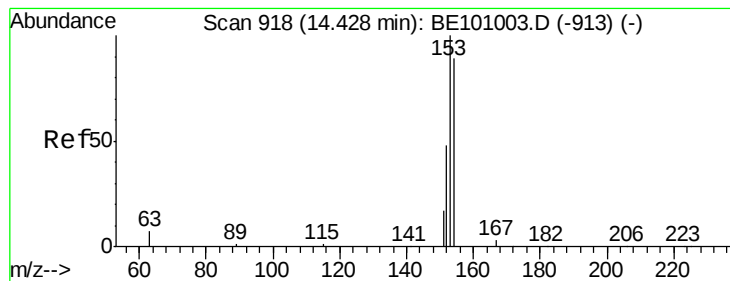

#17

Acenaphthene

Concen: 0.391 ng

RT: 14.41 min Scan# 916

Delta R.T. -0.02 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E


ClientSampleId :

PB126135BS




Tot Ion:	154	Resp:	8771
Ion	Ratio	Lower	Upper
154	100		
153	112.6	93.6	140.4
152	57.2	46.3	69.5

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



Abundance Ion 154.00 (153.70 to 154.70): E
Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E



#18

Fluorene

Concen: 0.373 ng


RT: 15.39 min Scan# 983

Delta R.T. -0.01 min



Lab File: BE101076.D


Acq: 16 Jan 2020 15:23

Tgt Ion:	166	Resp:	10579
Ion	Ratio	Lower	Upper
166	100		
165	98.4	79.8	119.8
167	12.8	11.0	16.6



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E





#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.09 min Scan# 1110

Delta R.T. 0.00 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E





ClientSampleId :

PB126135BS

Tot Ion:	188	Resp:	16559
Ion Ratio	Lower	Upper	
188	100		
94	0.0	0.0	0.0
80	11.5	10.8	16.2

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#20

4-Bromophenyl-phenylether

Concen: 0.373 ng




RT: 16.29 min Scan# 1050

Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion:	248	Resp:	3014
Ion Ratio	Lower	Upper	
248	100		
250	96.3	76.6	115.0
141	75.7	57.7	86.5









#21
Hexachlorobenzene
Concen: 0.402 ng
RT: 16.40 min Scan# 1058
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Instrument :
BNA_E
ClientSampleId :
PB126135BS

Tot Ion	Ratio	Lower	Upper
284	100		
142	42.0	34.0	51.0
249	35.4	28.2	42.4




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:34 PM



#22
Pentachlorophenol
Concen: 0.503 ng
RT: 16.75 min Scan# 1084
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
266	100		
264	69.0	61.0	91.4
268	65.2	58.5	87.7





#23

Phenanthrene

Concen: 0.385 ng

RT: 17.13 min Scan# 1113

Delta R.T. 0.00 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E





ClientSampleId :

PB126135BS

Tot Ion:	178	Resp:	17403
Ion	Ratio	Lower	Upper
178	100		
176	18.9	15.7	23.5
179	15.2	12.0	18.0

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#24

Anthracene

Concen: 0.414 ng




RT: 17.23 min Scan# 1120

Delta R.T. 0.00 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion:	178	Resp:	17658
Ion	Ratio	Lower	Upper
178	100		
176	18.4	14.8	22.2
179	15.4	12.4	18.6





#25

Fluoranthene-d10

Concen: 0.399 ng

RT: 19.12 min Scan# 1367

Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E





ClientSampleId :

PB126135BS

Tot Ion:	212	Resp:	91776
Ion Ratio	Lower	Upper	
212	100		
106	3.3	2.6	3.8
104	1.9	1.4	2.0

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#26

Fluoranthene

Concen: 0.396 ng




RT: 19.15 min Scan# 1373


Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion:	202	Resp:	22414
Ion Ratio	Lower	Upper	
202	100		
101	11.8	9.6	14.4
203	16.5	13.8	20.6









#27
Chrysene-d12
Concen: 0.400 ng
RT: 21.27 min Scan# 1622
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Instrument :
BNA_E
ClientSampleId :
PB126135BS

Tot Ion	Ratio	Lower	Upper
240	100		
120	12.8	8.6	13.0
236	28.1	22.2	33.4




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:34 PM



#28
Pyrene
Concen: 0.390 ng
RT: 19.51 min Scan# 1435
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
202	100		
200	21.2	17.0	25.4
203	17.5	13.8	20.6









#29
 Terphenyl-d14
 Concen: 0.381 ng
 RT: 19.73 min Scan# 1473
 Delta R.T. -0.01 min
 Lab File: BE101076.D
 Acq: 16 Jan 2020 15:23

Instrument :
 BNA_E
 ClientSampleId :
 PB126135BS

Tot Ion	Ratio	Lower	Upper
244	100		
212	33.5	27.2	40.8
122	12.8	9.8	14.8




Manual Integrations
 APPROVED

mohammad
 1/17/2020 2:10:34 PM



#30
 Benzo(a)anthracene
 Concen: 0.416 ng
 RT: 21.26 min Scan# 1621
 Delta R.T. -0.00 min
 Lab File: BE101076.D
 Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
228	100		
226	26.0	22.7	34.1
229	20.4	15.5	23.3





#31

Chrysene

Concen: 0.416 ng

RT: 21.31 min Scan# 1625

Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E





ClientSampleId :

PB126135BS

Tot Ion:	228	Resp:	28636
Ion Ratio	Lower	Upper	
228	100		
226	30.4	23.5	35.3
229	20.2	16.7	25.1

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.545 ng




RT: 21.20 min Scan# 1616

Delta R.T. -0.00 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion:	149	Resp:	42082
Ion Ratio	Lower	Upper	
149	100		
167	6.6	5.2	7.8
279	0.8	0.8	1.2





#33

Indeno(1,2,3-cd)pyrene

Concen: 0.495 ng

RT: 26.23 min Scan# 2858

Delta R.T. -0.02 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E





ClientSampleId :

PB126135BS

Tot Ion:	276	Resp:	26951
Ion Ratio	Lower	Upper	
276	100		
138	25.1	16.1	24.1#
277	24.4	18.1	27.1

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM



#34

Perylene-d12

Concen: 0.400 ng




RT: 23.69 min Scan# 2151


Delta R.T. -0.01 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Tgt Ion:	264	Resp:	21195
Ion Ratio	Lower	Upper	
264	100		
260	23.1	20.3	30.5
265	27.7	27.0	40.4









#35
Benzo(b)fluoranthene
Concen: 0.338 ng
RT: 22.95 min Scan# 1943
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Instrument :
BNA_E
ClientSampleId :
PB126135BS

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.1	18.5	27.7
125	11.9	9.5	14.3




Manual Integrations
APPROVED


mohammad
1/17/2020 2:10:34 PM



#36
Benzo(k)fluoranthene
Concen: 0.372 ng m
RT: 23.00 min Scan# 1956
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.6	18.9	28.3
125	19.3	10.1	15.1#









#37
Benzo(a)pyrene
Concen: 0.386 ng
RT: 23.58 min Scan# 2120
Delta R.T. -0.01 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Instrument :
BNA_E
ClientSampleId :
PB126135BS

Tot Ion	Ratio	Lower	Upper
252	100		
253	23.5	19.4	29.2
125	13.7	11.8	17.6




Manual Integrations
APPROVED




mohammad
1/17/2020 2:10:34 PM



#38
Dibenzo(a,h)anthracene
Concen: 0.401 ng
RT: 26.26 min Scan# 2866
Delta R.T. -0.02 min
Lab File: BE101076.D
Acq: 16 Jan 2020 15:23

Tgt Ion	Ratio	Lower	Upper
278	100		
139	19.5	15.0	22.4
279	24.8	22.6	33.8





#39

Benzo(a,h,i)perylene

Concen: 0.372 ng

RT: 27.01 min Scan# 3075

Delta R.T. -0.02 min

Lab File: BE101076.D

Acq: 16 Jan 2020 15:23

Instrument :

BNA_E

ClientSampleId :

PB126135BS

Tot Ion:	276	Resp:	24167
Ion Ratio	Lower	Upper	
276	100		
277	25.0	19.4	29.2
138	23.0	17.9	26.9

Manual Integrations
APPROVED

mohammad
1/17/2020 2:10:34 PM

