


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_E\DATA\BE011620\  
 Data File : BE101069.D  
 Acq On : 16 Jan 2020 9:41  
 Operator : JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE010820.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jan 08 18:36:25 2020

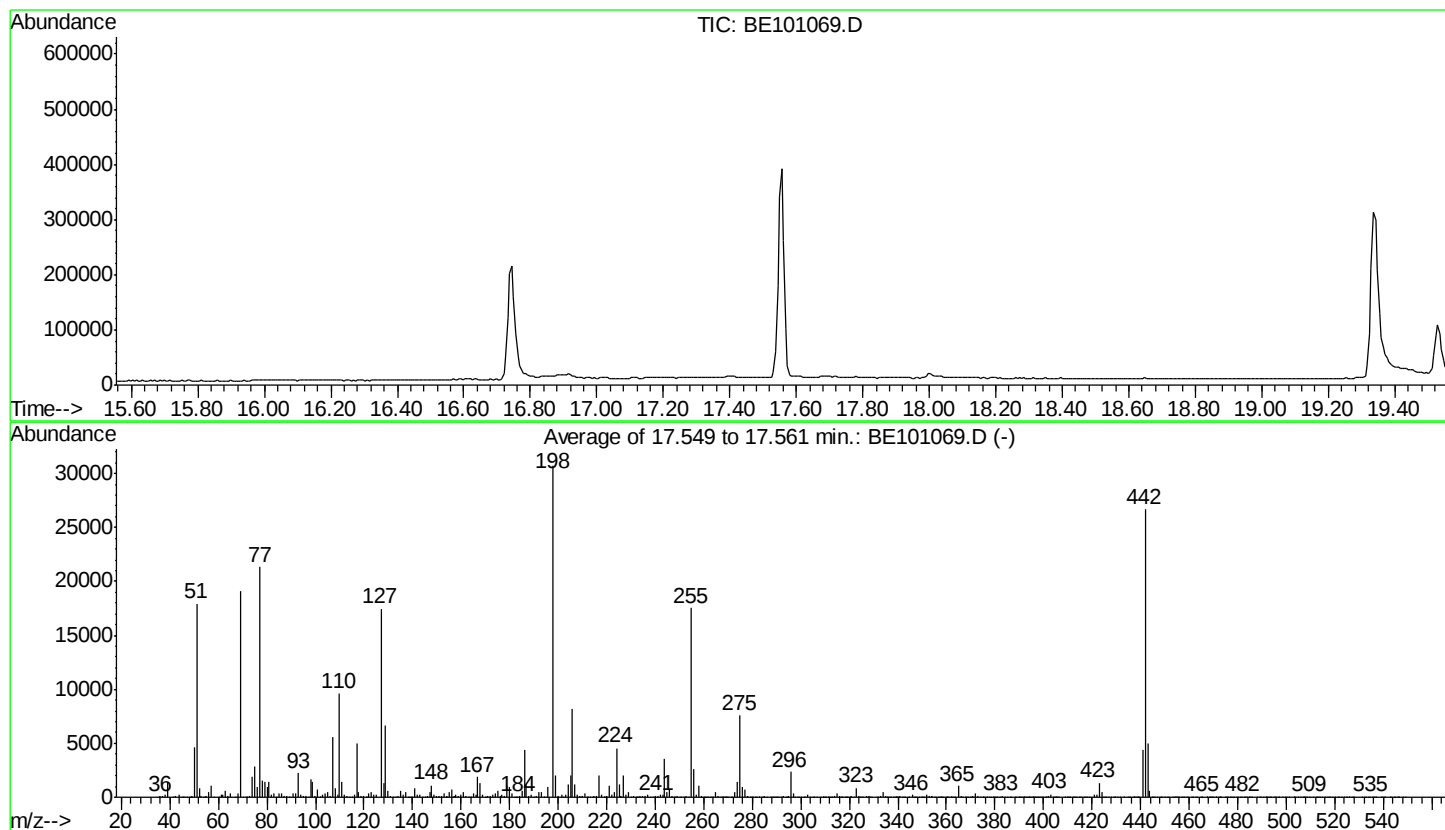

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2540

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 58.3      | 17928   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 309     | PASS             |
| 69          | 198          | 0.00         | 100          | 62.3      | 19134   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 51      | PASS             |
| 127         | 198          | 10           | 80           | 56.9      | 17485   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 30735   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 2043    | PASS             |
| 275         | 198          | 10           | 60           | 24.6      | 7547    | PASS             |
| 365         | 198          | 1            | 100          | 3.4       | 1035    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.3      | 4387    | PASS             |
| 442         | 198          | 50           | 100          | 86.8      | 26664   | PASS             |
| 443         | 442          | 15           | 24           | 18.7      | 4975    | PASS             |