
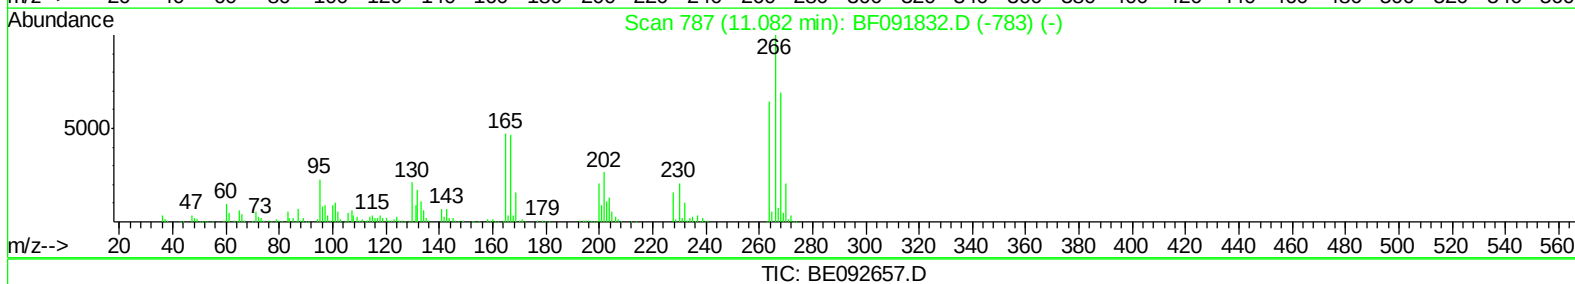
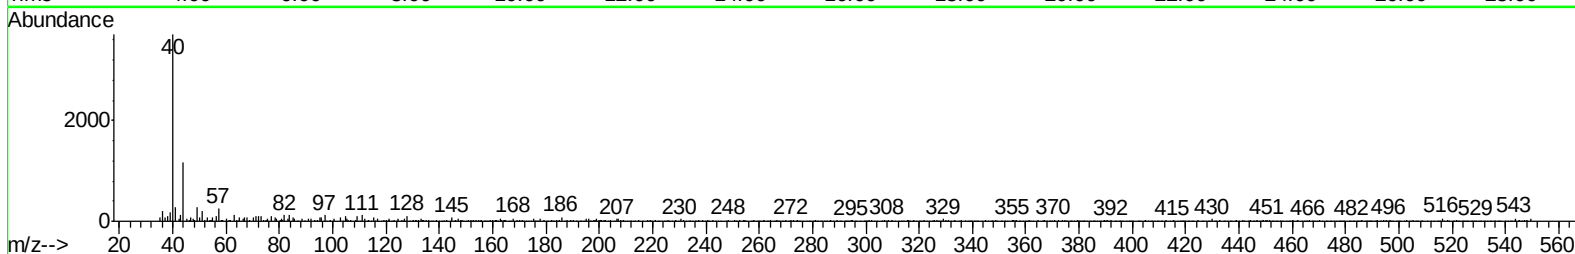


Data Path : Z:\HPCHEM1\BNA_E\Data\BE011917\
Data File : BE092657.D
Acq On : 19 Jan 2017 13:09
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 04:23:38 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

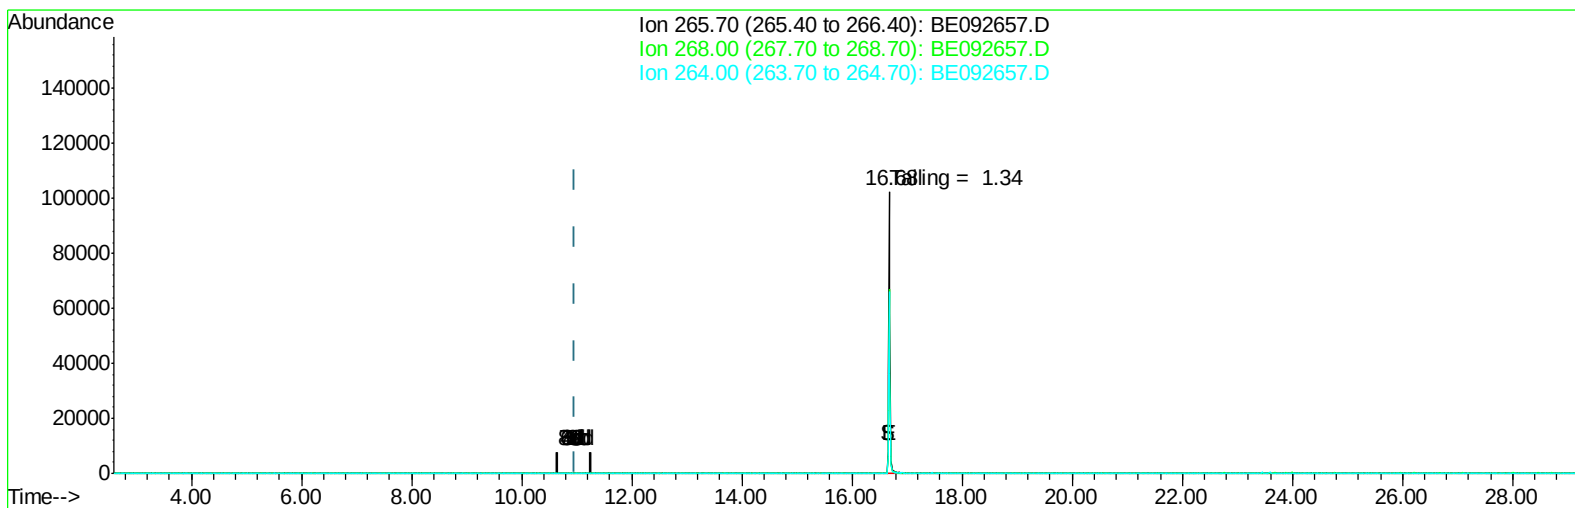

TIC: BE092657.D

(69) Pentachlorophenol (C)




11.001min (+0.028) 46.80ng

response 12

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	26.67#
264.00	62.90	120.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE011917\
Data File : BE092657.D
Acq On : 19 Jan 2017 13:09
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 20 04:23:38 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 06 15:43:51 2017
Response via : Initial Calibration

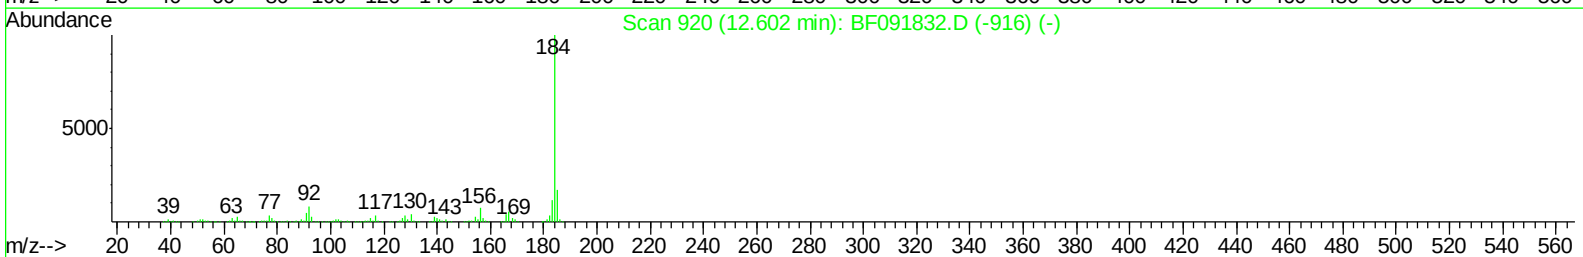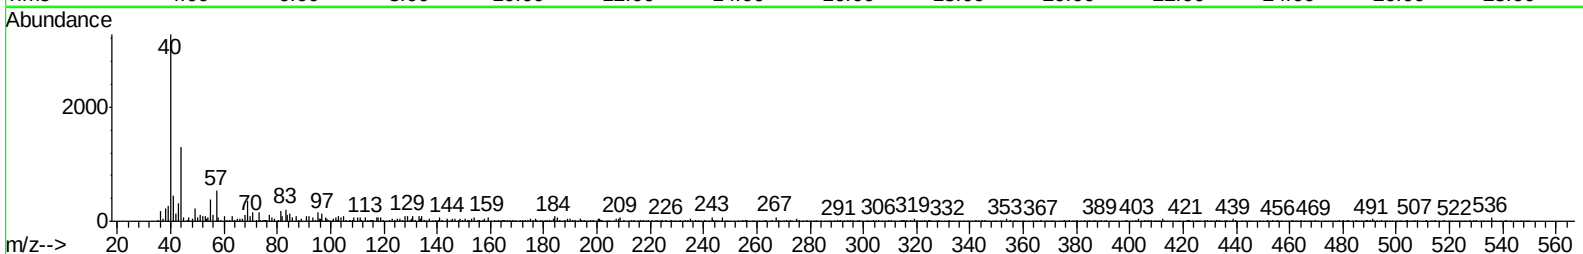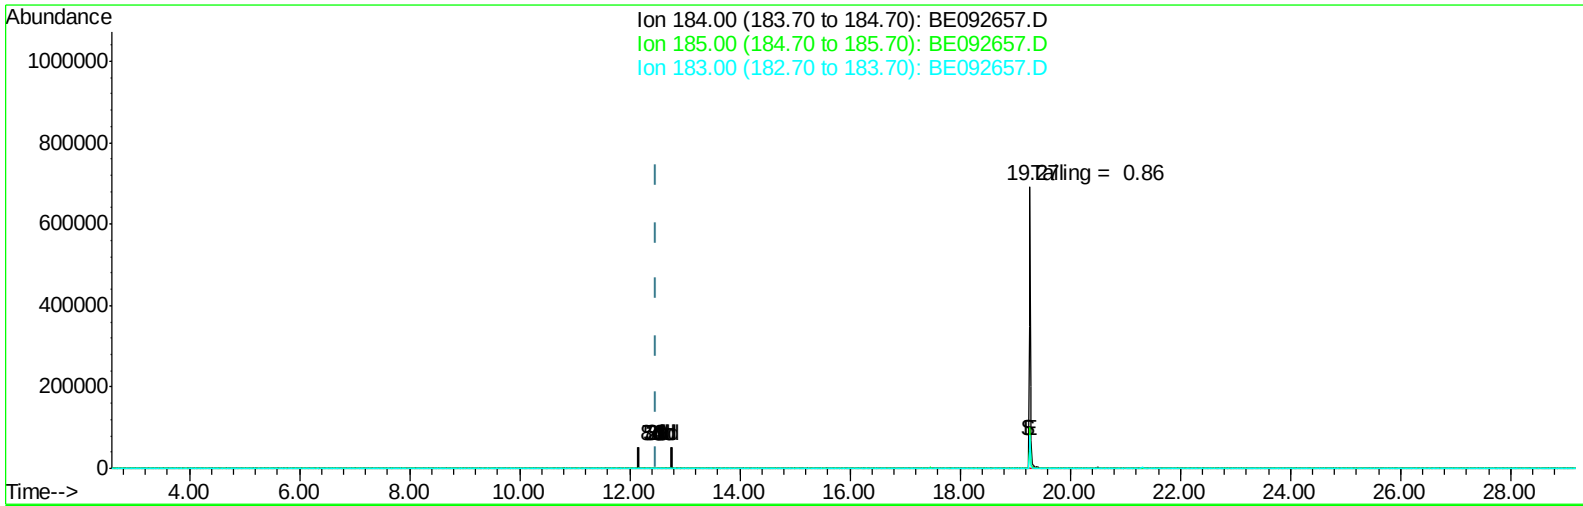

TIC: BE092657.D

(76) Benzidine

12.558min (+0.065) 53.24ng

response 52

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	86.36#
183.00	11.50	57.95#
0.00	0.00	0.00