


Data Path : Z:\HPCHEM1\BNA E\DATA\BE011917\
 Data File : BE092657.D
 Acq On : 19 Jan 2017 13:09
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 17 10:14:01 2017

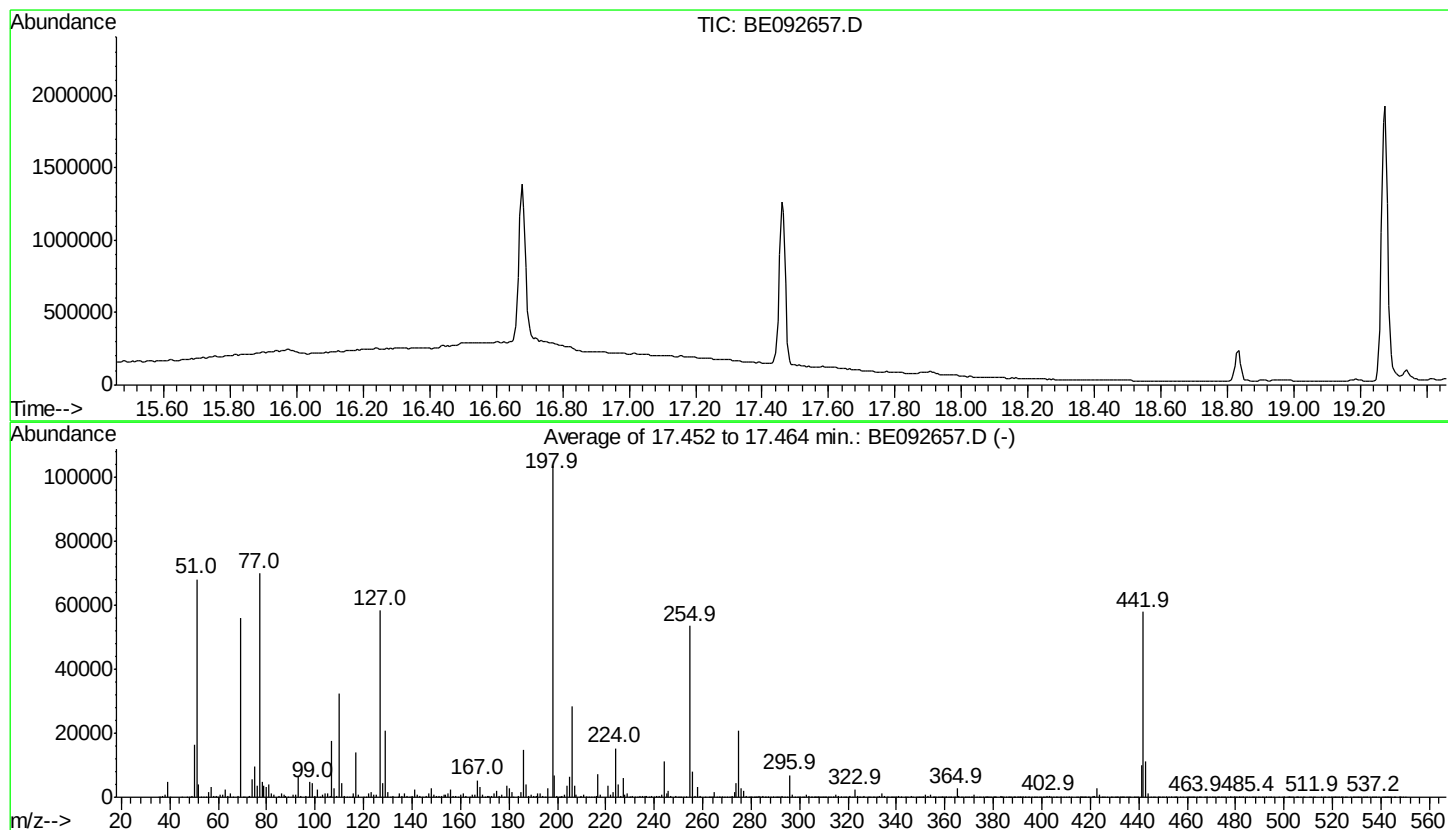

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.7	68066	PASS
68	69	0.00	2	0.9	521	PASS
69	198	0.00	100	54.0	55958	PASS
70	69	0.00	2	0.4	210	PASS
127	198	10	80	56.2	58302	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	103669	PASS
199	198	5	9	6.4	6655	PASS
275	198	10	60	20.1	20799	PASS
365	198	1	100	2.6	2715	PASS
441	442	0.01	24	17.4	10087	PASS
442	198	50	100	55.9	57902	PASS
443	442	15	24	19.2	11124	PASS