

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012018\
 Data File : BE095088.D
 Acq On : 20 Jan 2018 14:10
 Operator : SJ/JU
 Sample : PB105813BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 22 04:30:44 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE011918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 22 04:29:25 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.46	152	4392	0.40	ng/ul	0.00
2) Naphthalene-d8	11.28	136	14632	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.04	164	9431	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.73
16) Chrysene-d12	21.83	240	19631	0.40	ng/ul	0.00
20) Perylene-d12	24.32	264	1087617	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.84	152	8087	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.72	212	21661	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.07	202	2660	0.037	ng/ul#	Ovalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012018\
Data File : BE095088.D
Acq On : 20 Jan 2018 14:10
Operator : SJ/JU
Sample : PB105813BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 22 04:30:44 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE011918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 22 04:29:25 2018
Response via : Initial Calibration

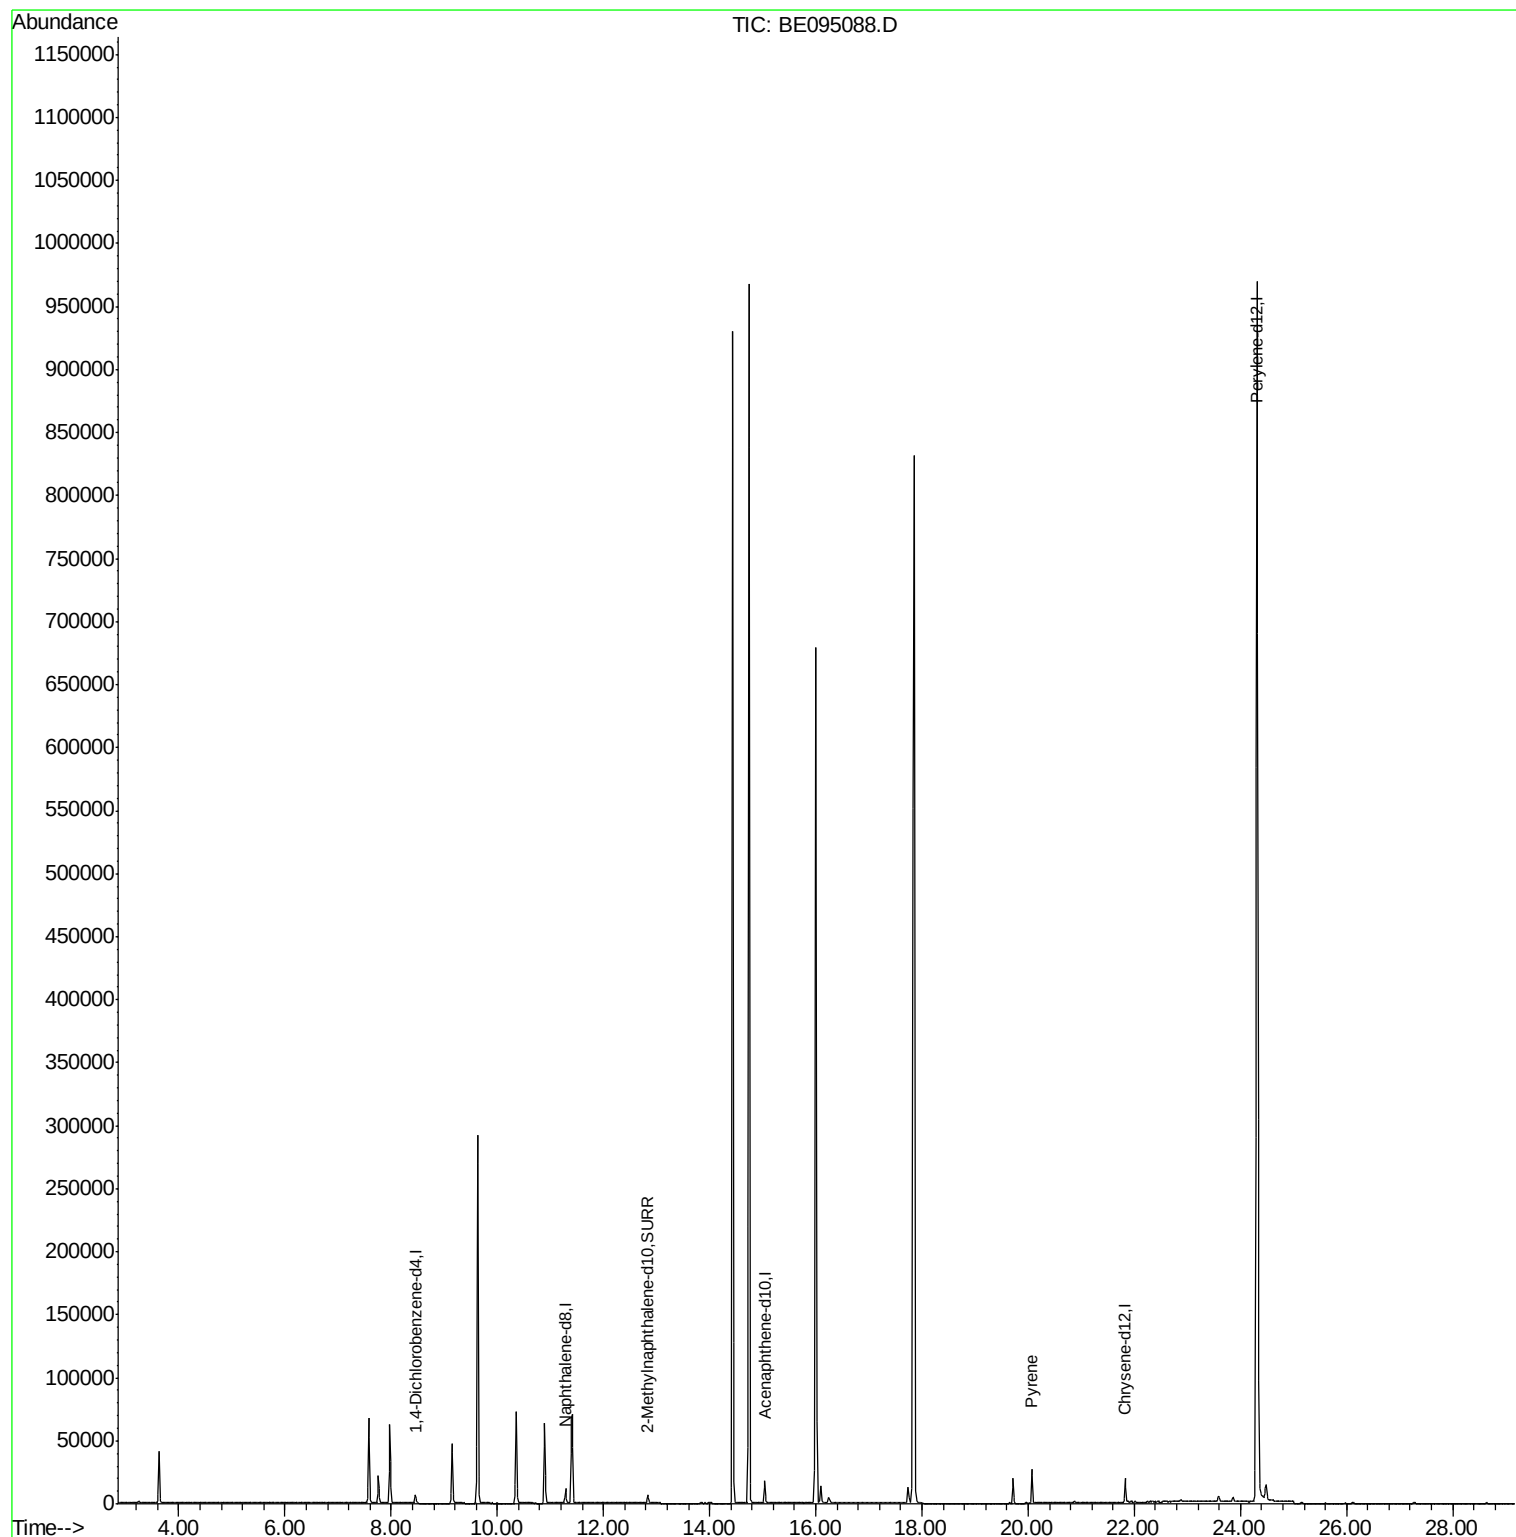

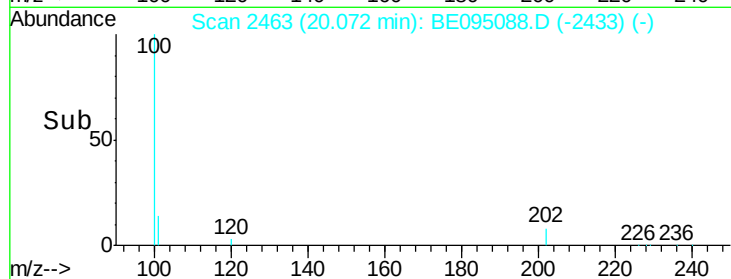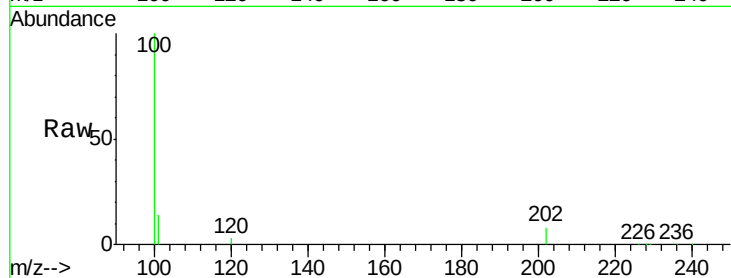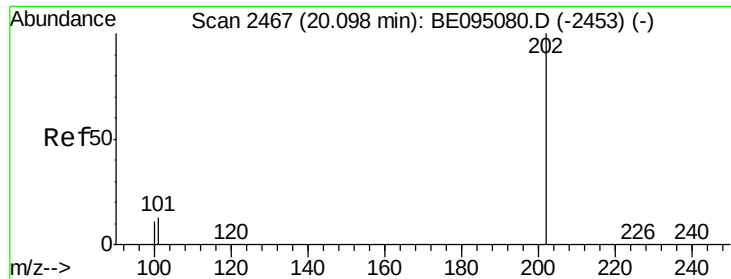

#17

Pvrene

Concen: 0.037 ng/ul

RT: 20.07 min Scan# 2463

Delta R.T. -0.03 min

Lab File: BE095088.D

Acq: 20 Jan 2018 14:10

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 202 Resp: 2660

Ion Ratio Lower Upper

202 100

101 163.7 18.2 27.4#

100 1178.1 15.6 23.4#

