
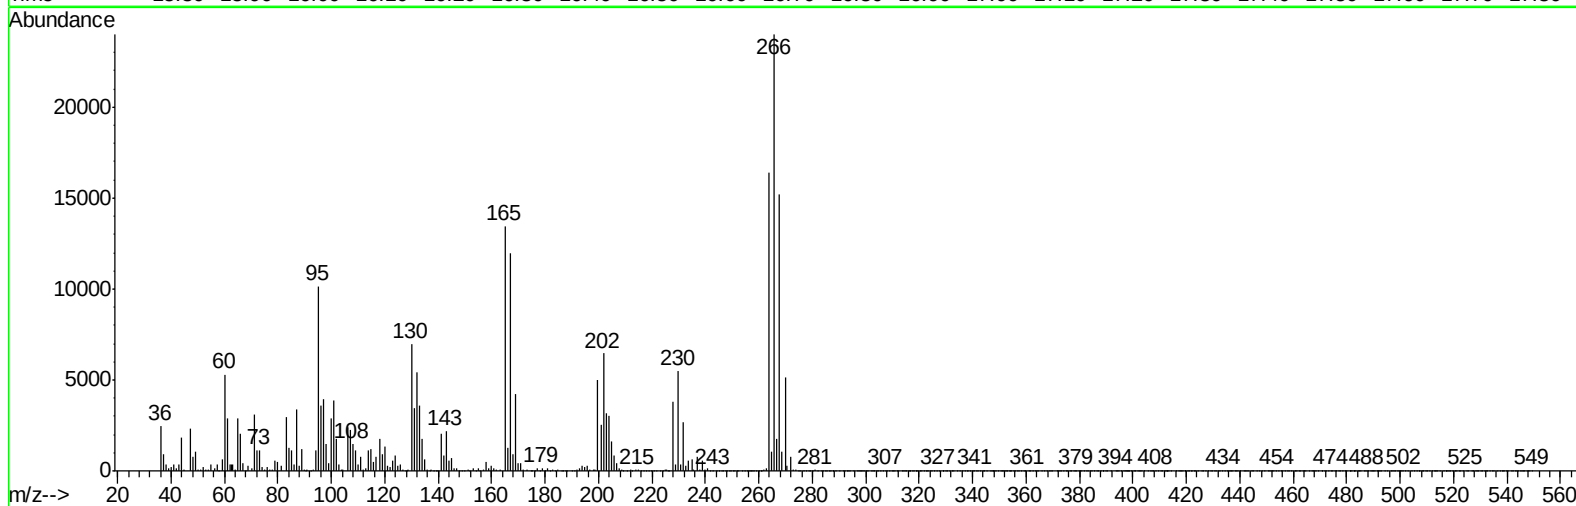


Data File : BE101103.D
Acq On : 21 Jan 2020 8:59
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 08:39:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 18:36:25 2020
Response via : Initial Calibration

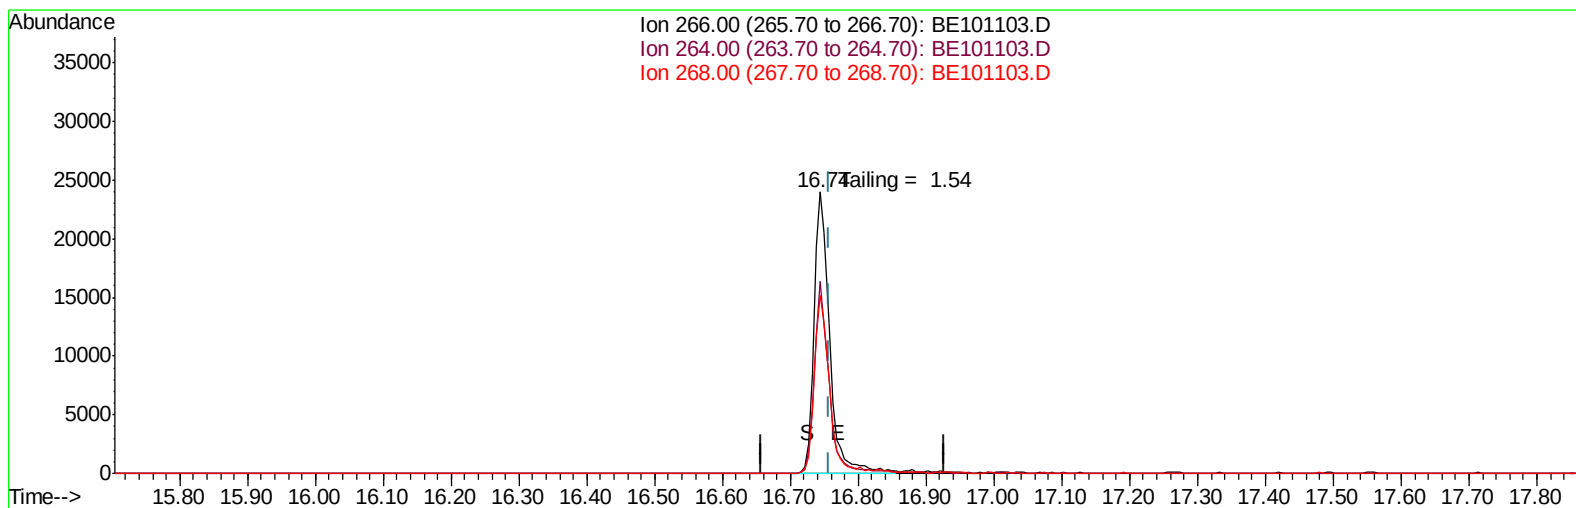

TIC: BE101103.D

(22) Pentachlorophenol

16.744min (-0.014) 4678.32ng

response 37657

Ion	Exp%	Act%
266.00	100	100
264.00	76.20	68.33
268.00	73.10	63.30
0.00	0.00	0.00