
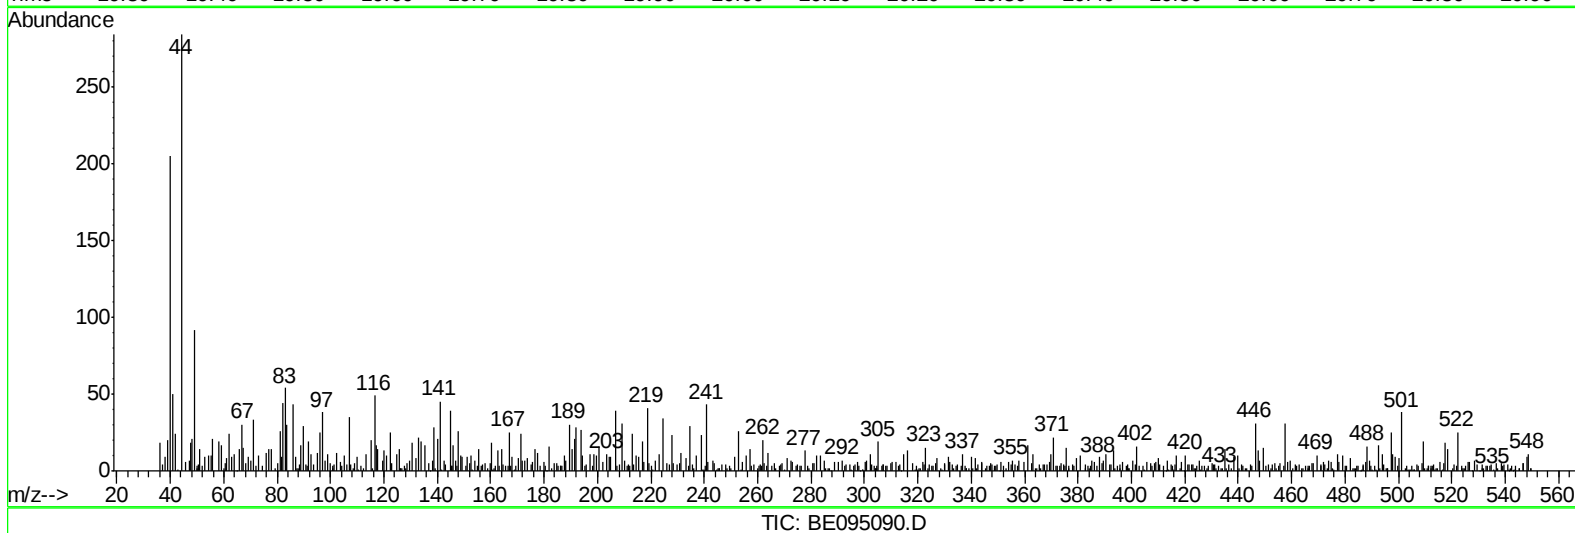


Data Path : Z:\HPCHEM1\BNA E\DATA\BE012318\
Data File : BE095090.D
Acq On : 23 Jan 2018 10:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 02:58:21 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 00:43:41 2018
Response via : Initial Calibration

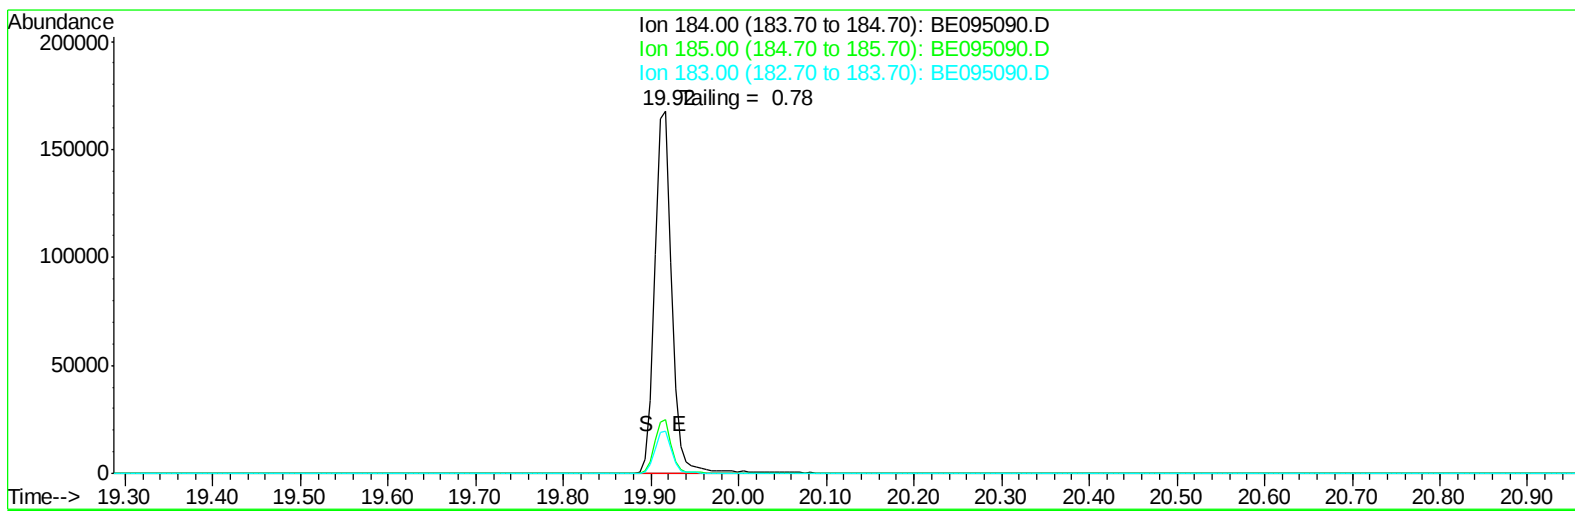

(76) Benzidine



12.549min (-0.026) 42.53ng

response 10

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	30.00#
183.00	11.60	20.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE012318\
Data File : BE095090.D
Acq On : 23 Jan 2018 10:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 24 02:58:21 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF012218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 23 00:43:41 2018
Response via : Initial Calibration

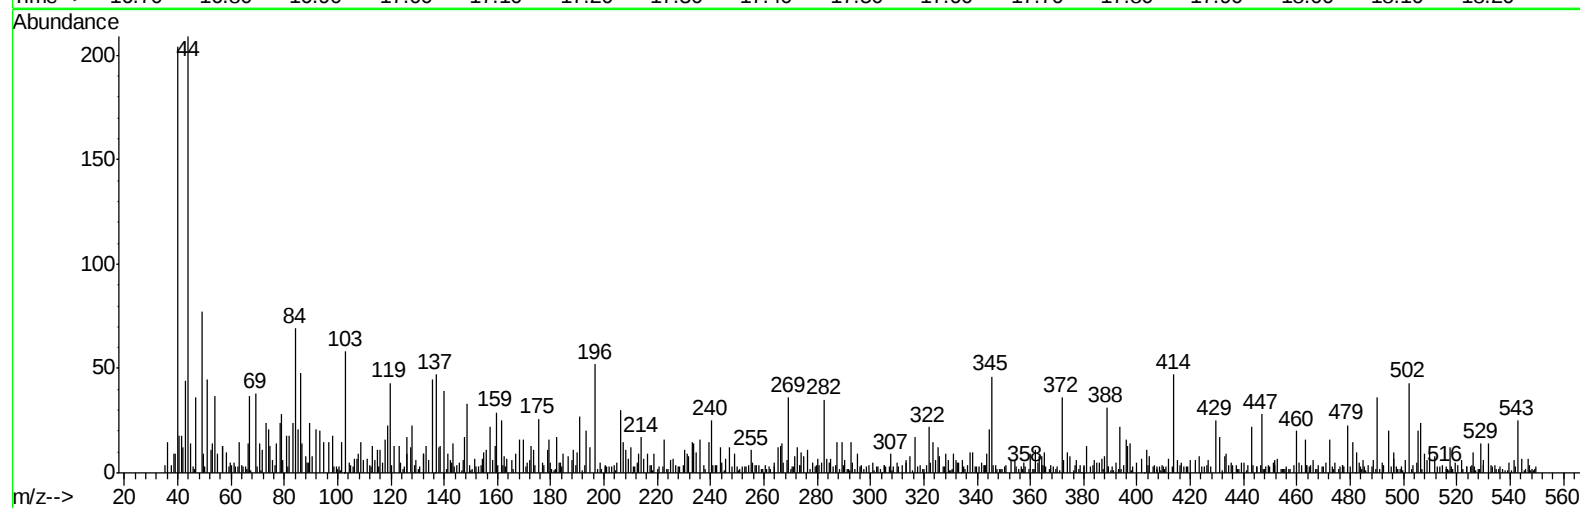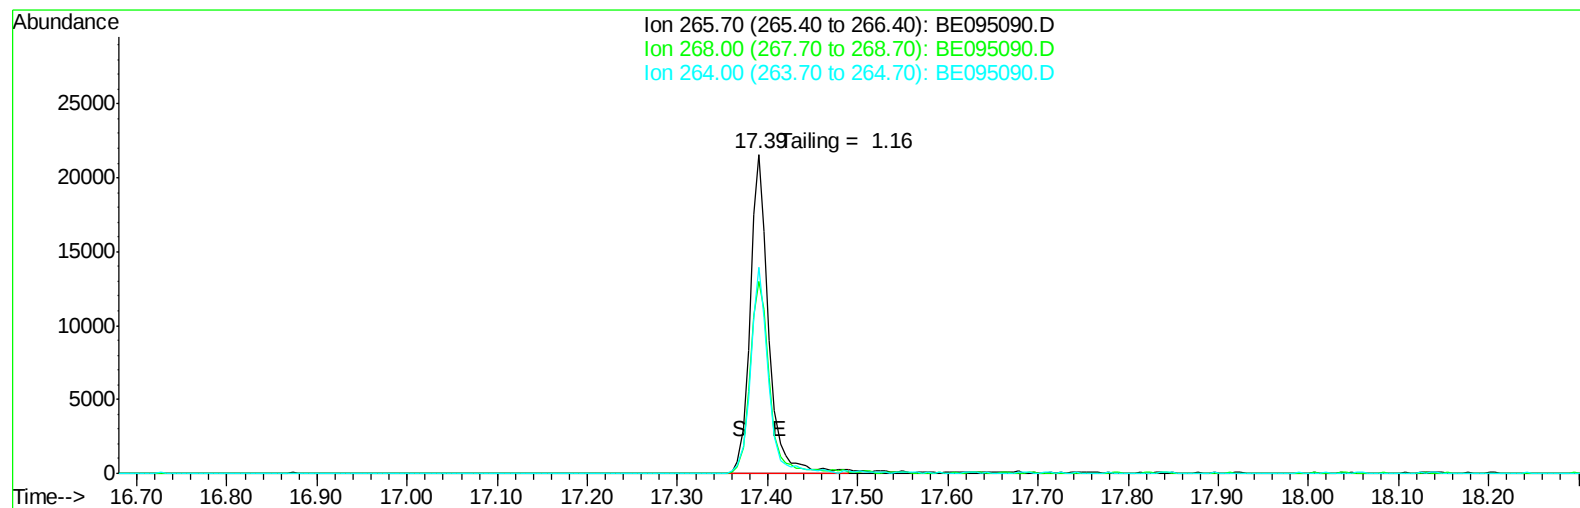

TIC: BE095090.D

(69) Pentachlorophenol (C)

10.998min (-0.048) 142.30ng

response 18

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	24.00#
264.00	61.90	32.00#
0.00	0.00	0.00