


Data Path : U:\HPCHEM1\BNA E\DATA\BE012318\
 Data File : BE095090.D
 Acq On : 23 Jan 2018 10:43
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE012318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 23 15:47:25 2018

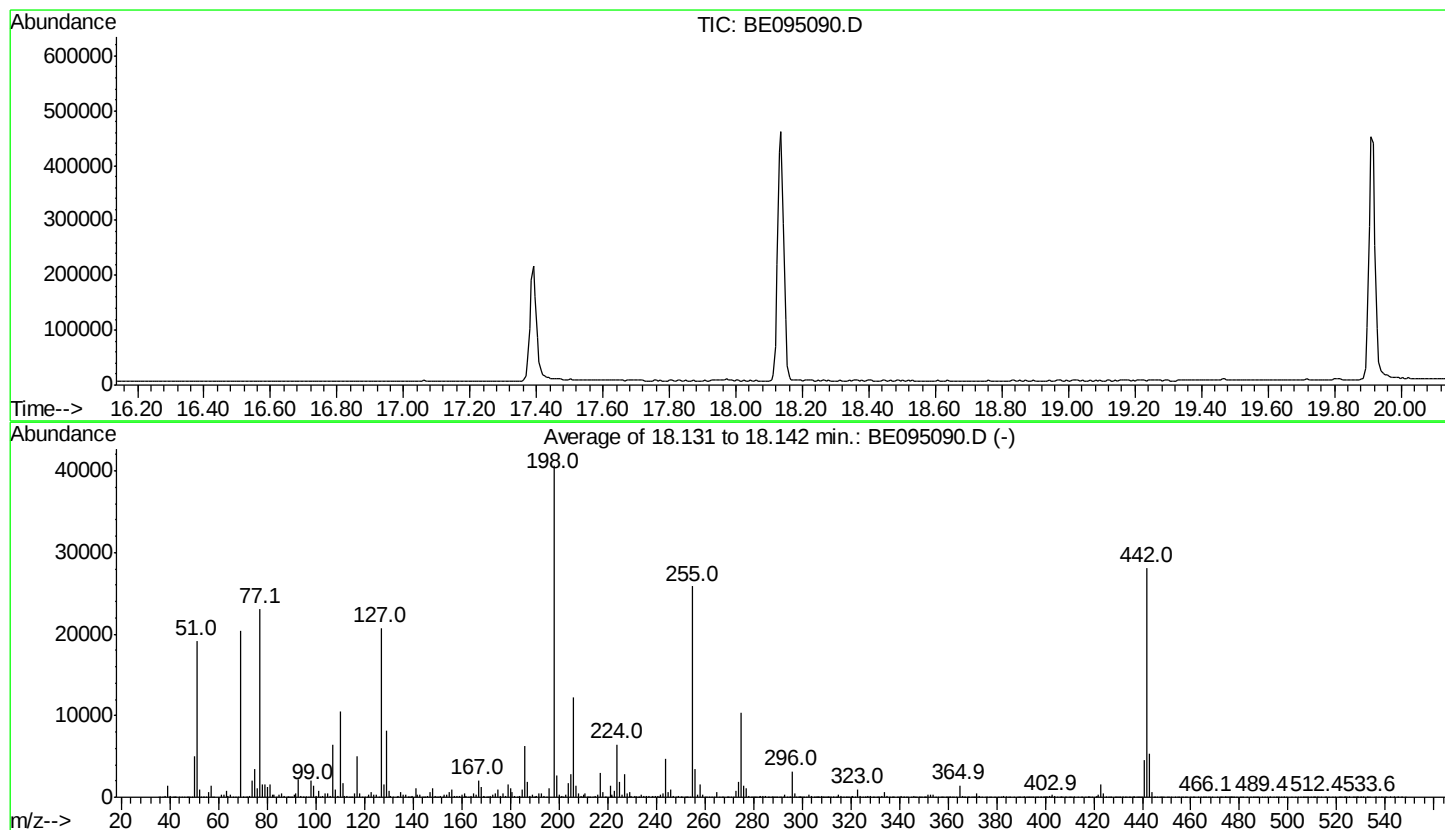

AutoFind: Scans 2645, 2646, 2647; Background Corrected with Scan 2637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	19151	PASS
68	69	0.00	2	0.4	82	PASS
69	198	0.00	100	50.2	20388	PASS
70	69	0.00	2	0.3	57	PASS
127	198	10	80	51.0	20722	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40650	PASS
199	198	5	9	6.8	2750	PASS
275	198	10	60	25.6	10406	PASS
365	198	1	100	3.6	1445	PASS
441	442	0.01	24	16.1	4542	PASS
442	198	50	100	69.3	28154	PASS
443	442	15	24	19.1	5371	PASS