


Data Path : Z:\HPCHEM1\BNA E\Data\BE012417\
 Data File : BE092670.D
 Acq On : 24 Jan 2017 17:55
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 17 10:14:01 2017

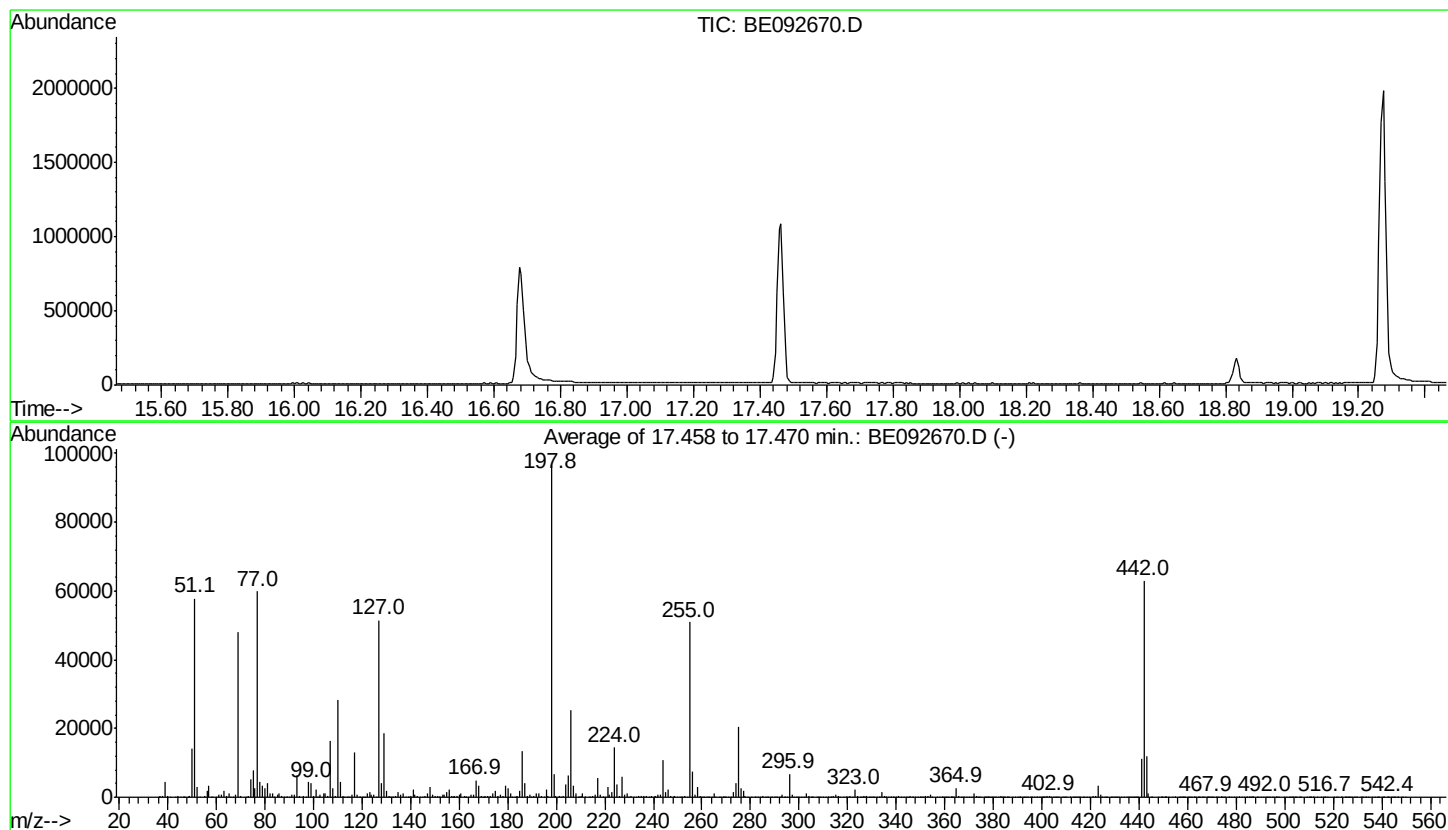

AutoFind: Scans 2531, 2532, 2533; Background Corrected with Scan 2521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.0	57861	PASS
68	69	0.00	2	1.7	807	PASS
69	198	0.00	100	49.8	48036	PASS
70	69	0.00	2	0.5	263	PASS
127	198	10	80	53.5	51566	PASS
197	198	0.00	2	0.3	250	PASS
198	198	100	100	100.0	96445	PASS
199	198	5	9	6.9	6655	PASS
275	198	10	60	21.3	20534	PASS
365	198	1	100	2.9	2781	PASS
441	442	0.01	24	17.7	11148	PASS
442	198	50	100	65.4	63042	PASS
443	442	15	24	18.9	11926	PASS